

County of San Luis Obispo Public Health Laboratory

Test Catalog



2191 Johnson Avenue, San Luis Obispo, CA 93401
Telephone: (805) 781-5512
Fax: (805) 781-1023

Hours

Monday to Friday: 8 am to 5 pm
Weekends: On-call ([805]-305-8188)

Laboratory Director: Glen M. Miller, PhD, HCLD (ABB)

Accreditations

CLIA: 05D0695770
CDPH Laboratory License: CDPH-0001260
ELAP: 2114
Federal Tax ID: 956000939
NPI: 1437103983

Table of Contents

- I. Contact information
- II. Laboratory requisitions
- III. Laboratory test information and collection instructions
 - a. Bacteriology test information
 - b. Bacteriology specimen collection
 - 1. Primary culture
 - 2. Carba-R assay
 - 3. *Neisseria gonorrhoeae* culture
 - 4. *Streptococcus* primary culture
 - 5. Stool culture
 - 6. Urine culture
 - c. Molecular test information
 - d. Molecular specimen collection
 - 1. *Chlamydia, Gonorrhea, Trichomonas, and Mycoplasma genitalium* NAAT testing
 - 2. Mumps PCR: Buccal swab
 - 3. Poxvirus PCR: Lesion swab
 - 4. Respiratory testing: Bronchial alveolar lavage or tracheal aspirate
 - 5. Respiratory testing: Nasopharyngeal aspirate
 - 6. Respiratory testing: Nasopharyngeal (NP) swab
 - 7. Respiratory testing: Throat swab
 - 8. Stool collection: GP panel and norovirus testing
 - 9. Stool collection: Norovirus testing
 - 10. Varicella zoster and Herpes: Lesion swabs
 - e. Mycobacteriology test information
 - f. Mycobacteriology specimen collection
 - 1. Sputum
 - 2. Cerebrospinal fluid
 - 3. Quantiferon Plus
 - g. Mycology test information
 - h. Mycology specimen collection
 - i. Parasitology test information
 - j. Parasitology specimen collection
 - 1. Blood smear for parasites
 - 2. Pinworm collection
 - 3. Stool collection: Ova and parasites

- k. Serology test information
 - l. Serology specimen collection
 - 1. Blood lead testing
 - 2. Serum
 - m. Sexually-transmitted infection test information
 - n. Sexually-transmitted infection specimen collection
 - o. Virology test information
 - p. Virology specimen collection
 - 1. Animals for rabies testing
 - q. Water and shellfish test information
 - r. Water and shellfish specimen collection
 - 1. Water collection in a 100 mL Idexx bottle
 - 2. Water collection in a 120 mL sterile Click Seal bottle
 - 3. Water collection in a sterile Nalgene bottle
- IV. Reportable diseases

I. Contact information

County of San Luis Obispo Public Health Laboratory

2191 Johnson Avenue
San Luis Obispo, CA 93401
Phone: (805) 781-5507
Fax: (805) 781-1023

Laboratory Director

Glen M. Miller, PhD, HCLD
Phone: (805) 781-5512
Email: gmmiller@co.slo.ca.us

Supervising Public Health Microbiologist

Lucia Martinez
Phone: (805) 781-5509
Email: lmartinez@co.slo.ca.us

Microbiologist on call (weekends)

Phone: (805) 305-8188

County of San Luis Obispo Infectious Diseases

Phone: (805) 781-5500
Fax: (805) 781-5543

II. Laboratory requisitions
 a. Requisition for clinical specimens



**COUNTY OF SAN LUIS OBISPO
 PUBLIC HEALTH LABORATORY**
 2191 Johnson Avenue, San Luis Obispo, CA 93401
 Ph: 805-781-5507 FAX: 805-781-1023
www.sloPublicHealth.org/lab
 CLIA: 05D0695770

THIS SPACE RESERVED FOR PUBLIC HEALTH LAB USE

PATIENT (or affix patient label below)		
Last Name	First Name	Middle Initial
Medical record #		
Residential Address <input type="checkbox"/> Same as Submitter Location		
City	State	Zip
DOB	<input type="checkbox"/> Male <input type="checkbox"/> Female <input type="checkbox"/> Other:	
Phone	Pregnancy Status	
Race	Ethnicity	
By signing here, the patient consents to be notified of results via text:		

SUBMITTER (Lab/Clinic/Medical Group)		
Account #		
Submitter Name		
Street Address		
City	State	Zip
Phone	Fax	
Name of Contact		
Ordering/Supervising Physician		
Signature of Physician or Authorized Representative (must be legible)		

SPECIMEN	
Collection Date	Collection Time
ICD-10 Codes (Include codes for Urine & Herpes cultures for FPACT patients) Codes	
CLINICAL HISTORY (Optional except for Reportable Conditions)	
Date of Onset	Symptoms
Reason for Today's Visit	
<input type="checkbox"/> Case	<input type="checkbox"/> Contact <input type="checkbox"/> Carrier <input type="checkbox"/> TOC

BILLING	
Insurance (provide copy of front & back of insurance card AND demographics)	
Insurance ID#	
<input type="checkbox"/> CenCal Health <input type="checkbox"/> Medi-Cal <input type="checkbox"/> Medicare <input type="checkbox"/> FPACT <input type="checkbox"/> Other Insurance (please specify):	
Payment type (if NOT billed to Insurance)	
<input type="checkbox"/> VISA <input type="checkbox"/> MC <input type="checkbox"/> Check# _____ <input type="checkbox"/> Cash	
Card #	Exp. Date
Amount Paid \$	<input type="checkbox"/> Fee Waived (add reason under COMMENTS)

SPECIMEN SOURCE			
<input type="checkbox"/> Aspirate	<input type="checkbox"/> *Nails	<input type="checkbox"/> Sputum	<input type="checkbox"/> Urine (Aptima)
<input type="checkbox"/> Blood, Whole	<input type="checkbox"/> Nasal Swab (VTM)	<input type="checkbox"/> Stool	<input type="checkbox"/> Urine (Sterile Cup)
<input type="checkbox"/> Bronchial Wash	<input type="checkbox"/> Nasopharynx Swab (VTM)	<input type="checkbox"/> Throat Swab (VTM)	<input type="checkbox"/> Vaginal Swab
<input type="checkbox"/> Cervical Swab	<input type="checkbox"/> Rectal Swab	<input type="checkbox"/> Throat Swab	<input type="checkbox"/> Other Swab (specify type):
<input type="checkbox"/> CSF	<input type="checkbox"/> Serum	<input type="checkbox"/> *Tissue	<input type="checkbox"/> Other/Location (specify):
<input type="checkbox"/> *Fluid	<input type="checkbox"/> *Skin	<input type="checkbox"/> Urethral swab	*Specify location on body:

TEST ORDER (Numeric codes for lab use only and subject to change)			
STI, Blood, & Urine	Respiratory	Gastrointestinal & Parasites	Mycology & Rash
<input type="checkbox"/> Chlamydia NAAT 2750	<input type="checkbox"/> Acid Fast Culture/Smear 3545	<input type="checkbox"/> Gastro Pathogen PCR panel (GP) 6500	<input type="checkbox"/> Coccidioides immitis DNA Probe 3915
<input type="checkbox"/> Gonorrhea NAAT 2770	<input type="checkbox"/> AFB isolate for ID 3555	<input type="checkbox"/> Norovirus NAAT 6100	<input type="checkbox"/> Mycology culture for ID 3910
<input type="checkbox"/> Trichomonas NAAT 2850	<input type="checkbox"/> MTB complex NAAT 3530	<input type="checkbox"/> Stool culture-Standard 2200	<input type="checkbox"/> Mycology primary culture 3905
<input type="checkbox"/> Herpes Virus NAAT 6840	<input type="checkbox"/> Quantiferon Plus 8800	<input type="checkbox"/> Salmonella culture 2220	<input type="checkbox"/> Enterovirus NAAT 6300
<input type="checkbox"/> HCV antibody, qualitative 5800	<input type="checkbox"/> Influenza NAAT 51005	<input type="checkbox"/> Shigella culture 2230	<input type="checkbox"/> Measles NAAT 6180
<input type="checkbox"/> HIV antibody, serum 5500	<input type="checkbox"/> Pertussis NAAT 2120	<input type="checkbox"/> Campylobacter culture 2240	<input type="checkbox"/> Mumps NAAT 6170
<input type="checkbox"/> HIV antibody differentiation 5700	<input type="checkbox"/> Pneumonia PCR panel (PN) 6620	<input type="checkbox"/> E. coli Shiga toxin-producing culture 2250	<input type="checkbox"/> Varicella Zoster antibody 5100
<input type="checkbox"/> Syphilis screen serum: RPR 5035	<input type="checkbox"/> Respiratory PCR panel (RP) 6310	<input type="checkbox"/> Cyclospora 4045	<input type="checkbox"/> Varicella Zoster NAAT 6900
<input type="checkbox"/> Syphilis confirm serum: TPPA 5065	<input type="checkbox"/> SC2/Flu NAAT with RP reflex 51015	<input type="checkbox"/> Helminth & Arthropod 4020	Other
<input type="checkbox"/> Syphilis screen CSF: VDRL 5000	<input type="checkbox"/> SC2/Flu/RSV NAAT 52000	<input type="checkbox"/> Microsporidia 4060	<input type="checkbox"/> Bacterial isolate for ID 2085
<input type="checkbox"/> Urine culture & susceptibility 2065	<input type="checkbox"/> SARS-CoV-2 NAAT 6860	<input type="checkbox"/> Ova & Parasite panel 4025	<input type="checkbox"/> Blood lead 6150
	<input type="checkbox"/> SARS-CoV-2 WGS screen 6070	<input type="checkbox"/> Pinworm (Paddle) 4005	<input type="checkbox"/> Other (specify):

Note: Order of Influenza and SARS-CoV-2 NAATs to be assigned to 51000 (LAB USE ONLY) Alternate Order Codes:
Please contact the Laboratory for questions, reference specimens, and other tests.
 COMMENTS:

Req 100 Generic (04/13/2023)

b. Requisition for water samples



**COUNTY OF SAN LUIS OBISPO
PUBLIC HEALTH LABORATORY**
2191 Johnson Avenue, San Luis Obispo, CA 93401
Ph: 805-781-5507 Fax: 805-781-1023
www.sloPublicHealth.org/lab
ELAP: 2114

THIS SPACE RESERVED FOR PUBLIC HEALTH LAB USE

SAMPLE COLLECTION		
Sample ID # (you make this up, must also be on sample container)		
Sampling Location (wellhead/kitchen sink/etc.)		
Sampling Street Address		<input type="checkbox"/> Same as Submitter Location
City	State	ZIP
Comments:		

SUBMITTER		
Account #		
Submitter Name		
Submitter Street Address		
City	State	ZIP
Contact Name		<input type="checkbox"/> Same as Above
Phone (please print clearly)	Fax	
Email (please print clearly)		

SAMPLE COLLECTION	
Collection Date	Collection Time <input type="checkbox"/> AM <input type="checkbox"/> PM
Sample Collector Name (please print clearly)	
Sample Collector Signature	
Reason for Testing	<input type="checkbox"/> Routine <input type="checkbox"/> Survey <input type="checkbox"/> Replacement <input type="checkbox"/> Retest <input type="checkbox"/> Other
Free Residual Chlorine (if reported)	
Temperature Upon Receipt (°C) & Thermometer Number Used	

BILLING	
Send Invoice To	<input type="checkbox"/> Same as Above
Amount Paid	
\$	
<input type="checkbox"/> Visa #:	Exp. Date
<input type="checkbox"/> MC #:	
<input type="checkbox"/> Check #:	<input type="checkbox"/> Cash <input type="checkbox"/> Fee Waived

SAMPLE SOURCE			
<input type="checkbox"/> Drinking Water	<input type="checkbox"/> Pool/Spa Water	<input type="checkbox"/> Creek/Stream/Lake Water	<input type="checkbox"/> DI (deionized) Water
<input type="checkbox"/> Irrigation Water	<input type="checkbox"/> Hot Tub Water	<input type="checkbox"/> Dental Water	<input type="checkbox"/> Other (specify):

TEST ORDER	
<input type="checkbox"/> 8040 Total Coliforms/ <i>E. coli</i> -Bacterial Presence/Absence-Drinking Water Quality (SM 9223 Idexx Collert)	
<input type="checkbox"/> 8350 Total Coliforms/ <i>E. coli</i> , undiluted, Most Probable Number (SM 9223 Idexx Collert QuantTray)	
<input type="checkbox"/> 8910 Thermotolerant (Fecal) Coliforms MPN-A1 (SM 9221E A1 MTF)	<input type="checkbox"/> 8045 Heterotrophic Plate Count-HPC (SM 9215B)
<input type="checkbox"/> 8069 Salinity (Refractometry)	<input type="checkbox"/> 9300 Surface Sanitation Culture
<input type="checkbox"/> 8025 Total Coliforms/ <i>E. coli</i> , diluted, MPN (SM 9223 Idexx Collert QuantTray)	<input type="checkbox"/> Other (specify):
<input type="checkbox"/> 8010 Enterococci, diluted, MPN (SM 9230 Idexx Enterolert QuantTray)	

CUSTODY TRANSFER					
Relinquished By	Date	Time	Received By	Date	Time
Relinquished By	Date	Time	Received By	Date	Time

Requisition 200 Environmental Updated 24 June 2022

c. Requisition for tick submissions



**SAN LUIS OBISPO COUNTY
PUBLIC HEALTH LABORATORY**

Ph: 805-781-5507 FAX: 805-781-1023
www.sloPublicHealth.org/lab
 2191 Johnson Avenue, San Luis Obispo, CA 93401
 CLIA : 05D0695770

THIS SPACE RESERVED FOR PUBLIC HEALTH LAB USE

ANIMAL/BIRD/INSECT TESTING				SUBMITTER			
Sample Control # N/A				Account 152511H			
Species				Submitter Name SAN LUIS OBISPO COUNTY PUBLIC HEALTH			
Color/Markings				Street Address 2191 JOHNSON AVE			
Date Died/Euthanized		Date Collected		City SAN LUIS OBISPO		State CA	ZIP 93401
DAS #				Name of Contact PH LAB			
<input type="checkbox"/> Pet	<input type="checkbox"/> Stray	<input type="checkbox"/> Wild	<input type="checkbox"/> Unknown	Phone 805-781-5507		FAX 805-781-1023	
Was suspect animal immunized for rabies? <input type="checkbox"/> Yes <input type="checkbox"/> No <input type="checkbox"/> Unknown				BILLING			
Type of Exposure: <input type="checkbox"/> Bite <input type="checkbox"/> Non-Bite <input type="checkbox"/> Unknown <input type="checkbox"/> Other (Describe Below):				<input type="checkbox"/> Send Invoice To			
OWNER				Amount Paid			
Name N/A				<input type="checkbox"/> Check #	<input type="checkbox"/> Cash	<input type="checkbox"/> Fee Waived	
Street Address				\$			
City				<input type="checkbox"/> VISA	<input type="checkbox"/> MC	Exp. Date	
State				Card #			
ZIP				TEST REQUEST			
Phone #1		Phone #2		<input type="checkbox"/> Routine <input type="checkbox"/> Urgent <input type="checkbox"/> Other (Specify):			
VICTIM (IF BITE OCCURRED)				SPECIMEN TYPE			
Name				<input type="checkbox"/> Head <input type="checkbox"/> Brain <input type="checkbox"/> Carcass <input type="checkbox"/> Other (Specify):			
Street Address			Sex	Comments:			
City		State	ZIP	TICK			
Phone #1		DOB					
DESCRIBE CONTACT							
TEST ORDER (ORDER CODE)							
<input type="checkbox"/> Rabies DFA (8000)				<input type="checkbox"/> Helminth & Arthropod (insect, spider, etc) Identification (4020)			
<input type="checkbox"/> Plague – <i>Yersinia pestis</i> (9100)				<input type="checkbox"/> Tick Identification (4015)			
<input type="checkbox"/> Anthrax – <i>Bacillus anthracis</i> (9100)				<input type="checkbox"/> West Nile Virus PCR (8150)			
<input type="checkbox"/> Tularemia – <i>Francisella tularensis</i> (9100)				<input type="checkbox"/> Other (Specify): Lyme Disease Testing (refer to Santa Clara)			
<input type="checkbox"/> Brucellosis – <i>Brucella</i> spp (9100)							
CUSTODY							
Relinquished By		Date	Time	Relinquished By		Date	Time
Received By		Date	Time	Received By		Date	Time

Tick Submittal Req 300 (12/2/2021)

III. Laboratory test information and collection instructions

a. Bacteriology test information

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Aeromonas culture (2310)	Culture and isolation of <i>Aeromonas</i> species from stool specimens	Stool	Stool collected in Cary-Blair or Amies transport media	Refrigerated (2–8°C): 4 days Room temp. (15–25°C): 2 days	No pathogen isolated	Daily	2 days	87046
Antibiotic susceptibility testing, urine isolate (2600)	Determination of susceptibility and resistance patterns for uropathogens isolated from culture	Urine	Urine collected in a sterile container, in Boritex Urine Preservative, or BD Vacutainer Urine Collection System	<u>Sterile container</u> : room temperature for 2 hours or refrigerated for 24 hours <u>Boritex</u> : room temperature for 72 hours <u>BD Vacutainer</u> : room temperature for 48 hours	Susceptible	Daily	Prelim: 1 day Final: 3 days	87184
Bacteriology primary culture (2025)	Culture and isolation of aerobic and anaerobic bacterial pathogens from primary specimens	Abscess or wound aspirate, biopsy material, swab of superficial wound, tissue sample, wound drainage fluid	<u>Aspirates/drainages</u> : fluid collected in a sterile container <u>Biopsies</u> : place in sterile tube with broth culture medium or saline <u>Swabs</u> : Collect into transport system with Stuart’s or Amies medium <u>Tissues</u> : Collect in sterile vial with saline or anaerobe transport vial	Specimens must be transported to the laboratory within 24 hours of collection, 4°C to 25°C	No pathogen isolated	Daily	Prelim: 1 day Final: Pathogen-specific but typically 3 days for most aerobic pathogens (then referral if needed)	87070

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Bacteriology isolate identification, set-up (2085)	Culture procedure for miscellaneous bacteria to set-up identification	Bacterial isolate	Bacteria inoculated onto slant medium	Bacteria-specific; must be viable upon receipt	Non-pathogenic bacteria	Daily	3 days to ID or referral	87077
Campylobacter culture (2240)	Culture and isolation of <i>Campylobacter</i> species from stool specimens	Stool	Stool collected in Cary-Blair or Amies transport media	Refrigerated (2–8°C): 4 days Room temp. (15–25°C): 2 days	No pathogen isolated	Daily	4 days	87046
Carba-R assay (2350)	Detection of beta-lactamase genes associated with carbapenem-non-susceptibility—IMP, VIM, NDM, KPC, and OXA-48—using the GeneXpert instrument	Bacterial isolates (Enterobacteriales, <i>A. baumannii</i> , or <i>P. aeruginosa</i>), rectal swabs, or perirectal swabs	<u>Isolates</u> : inoculated onto slant medium <u>Swabs</u> : collected into Cepheid collection device	<u>Isolates</u> : ambient or refrigerated but must be viable for subculturing <u>Swabs</u> : 15–28 °C for up to 5 days	No beta-lactamase genes detected	Daily	1 day	87150
<i>E. coli</i> shiga toxin-producing culture (225)	Culture and isolation of shiga toxin-producing <i>E. coli</i> from stool specimens	Stool	Stool collected in Cary-Blair or Amies transport media	Refrigerated (2–8°C): 4 days Room temp. (15–25°C): 2 days	No shiga toxins detected	Daily	3 days then referral if positive	87046

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
E. coli shiga toxin-producing isolate, confirmation (2080)	Shiga toxin characterization and serotyping of shiga toxin-producing <i>E. coli</i>	Isolate, GN broth, or MacConkey broth	GN or MacConkey broth inoculated with stool and incubated for 16-24 hours	<u>Isolate:</u> ambient, must be viable upon receipt <u>Broth culture:</u> refrigerated, must exhibit growth upon receipt (recommended within 14 days)	No shiga toxins detected	Daily	2 days then referral if positive	87070
Gram stain (2035)	Classification of bacteria based on form, size, and Gram reaction	Pure culture or specimen	Specimen dependent	Specimen dependent	No bacteria seen	Daily	1 day	87205
Legionella urinary antigen test (2400)	Rapid detection of <i>Legionella</i> serogroup 1 antigen from urine specimens	Urine	Urine from hospitalized patient in sterile container or container with boric acid preservative	<u>Ambient:</u> 24 hours <u>Refrigerated:</u> 14 days <u>Frozen:</u> 30 days	Presumptive negative	Daily	1 day	87426
MALDI-TOF MS bacterial ID (2460, 2470)	Identification of bacterial isolates using the mass and intensity distribution of protein profile from a Bruker MALDI Biotyper	Bacterial isolate	Bacteria inoculated onto slant medium	Bacteria-specific; must be viable upon receipt	Not applicable	Daily	1 day	87077

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Neisseria gonorrhoeae culture (2050)	Culture and isolation of <i>Neisseria gonorrhoeae</i> from primary specimens	Swab of urogenital, cervical, rectal, or oropharyngeal site	Dacron or rayon swab of site placed in Amies transport medium	Ambient for up to 48 hours	No pathogen isolated	Daily	3 days	87850
Neisseria gonorrhoeae culture confirmation (2040)	Identification of <i>Neisseria gonorrhoeae</i>	Bacterial isolate	Bacteria inoculated onto slant medium	Bacterium must be viable upon receipt	No pathogen identified	Daily	2 days	87077
Salmonella culture (2220)	Culture and isolation of <i>Salmonella</i> from stool	Stool	Stool collected in Cary-Blair or Amies transport media	Refrigerated (2–8°C): 4 days Room temp. (15–25°C): 2 days	No pathogen isolated	Daily	4 days	87045
Shigella culture (2230)	Culture and isolation of <i>Shigella</i> from stool	Stool	Stool collected in Cary-Blair or Amies transport media	Refrigerated (2–8°C): 4 days Room temp. (15–25°C): 2 days	No pathogen isolated	Daily	4 days	87045

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Shiga toxin EIA (2290)	Detection of shiga toxin 1 and 2 in stool specimens or broth culture	Stool	Stool collected in a sterile container, Cary-Blair media, or Amies transport media	<u>Unpreserved stool or stool in transport media (direct method)</u> ; refrigerated or frozen for up to 14 days <u>Unpreserved stool (broth method)</u> ; frozen for up to 14 days <u>Stool in transport media (broth method)</u> ; refrigerated for up to 5 days	No shiga toxins detected	Daily	1 day	87427
Stool culture isolate identification (2280)	Set-up procedure for identifying a bacterium isolated from stool	Bacterial isolate	Bacteria inoculated onto slant medium	Bacterium must be viable upon receipt	Non-pathogenic bacterium	Daily	2 days	87045
Streptococcus culture (2015)	Culture and isolation of beta-hemolytic streptococci from swab specimens	Rectal swab, throat swab, or vaginal swab	Swab collected into Amies transport medium	Ambient for up to 24 hours	Negative	Daily	1 day	87081

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Urine culture with colony count (2065)	Isolation and identification of uropathogens from urine specimens	Urine	Urine collected in a sterile container, in Boritex Urine Preservative, or BD Vacutainer Urine Collection System	<u>Sterile container</u> : room temperature for 2 hours or refrigerated for 24 hours <u>Boritex</u> : room temperature for 72 hours <u>BD Vacutainer</u> : room temperature for 48 hours	No growth in 24 hours	Daily	Prelim: 1 day Final: 3 days	87086
Vibrio culture	Culture and isolation of <i>Vibrio</i> species from stool	Stool	Stool collected in Cary-Blair or Amies transport media	Refrigerated (2–8°C): 4 days Room temp. (15–25°C): 2 days	No pathogen isolated	Daily	3 days	87046
Yersinia enterocolitica culture	Culture, isolation, and identification of <i>Y. enterocolitica</i> from stool	Stool	Stool collected in Cary-Blair or Amies transport media	Refrigerated (2–8°C): 4 days Room temp. (15–25°C): 2 days	No pathogen isolated	Daily	2 days	87046
Bacteriology panels								
Gastrointestinal PCR panel (6500)	Biofire PCR panel that detects 22 agents (viruses, bacteria, and parasites) that cause diarrhea	Stool	Stool in Cary-Blair transport medium (preferred), stool in a sterile container,	<u>Cary-Blair</u> : ambient or refrigerated for up to 4 days <u>Sterile container</u> : ambient for 2 hours	No pathogens detected	Daily	1 day	0097U

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Stool culture, comprehensive (3000)	Culture and isolation of <i>Salmonella</i> , <i>Shigella</i> , <i>Campylobacter</i> , Shiga toxin-producing <i>E. coli</i> , <i>Vibrio</i> species, <i>Aeromonas</i> species, and <i>Plesiomonas shigelloides</i>	Stool	Stool collected in Cary-Blair or Amies transport media	Refrigerated (2-8°C): 4 days Room temp. (15-25°C): 2 days	No pathogen isolated	Daily	4 days	87045, 87046
Stool culture, standard (2200)	Culture and isolation of for <i>Salmonella</i> , <i>Shigella</i> , <i>Campylobacter</i> , and Shiga toxin-producing <i>E. coli</i>	Stool	Stool collected in Cary-Blair or Amies transport media	Refrigerated (2-8°C): 4 days Room temp. (15-25°C): 2 days	No pathogen isolated	Daily	4 days	87045, 87046

TAT, turnaround time (estimated maximum time from specimen receipt to result, where the time is dependent upon day of receipt, testing schedule, and length of testing).

b. Bacteriology specimen collection

1. Primary culture

- a. Specimens include abscess or wound aspirate, biopsy material, swab of superficial wound, tissue sample, wound drainage fluid

Specimen

Abscess or wound aspirate in a sterile container

1. Disinfect the skin surface with 70% alcohol. Allow it to dry.
2. Aspirate specimen directly into a syringe. Remove air from syringe.
3. Aseptically transfer aspirate into a sterile container.
4. If the specimen must be transported in the syringe, replace the needle with a sterile Leur cap.
5. If unable to aspirate and swab is used, pass a swab deep into the lesion and firmly sample the lesion's advancing edge. Place swab into Amies transport medium for aerobes.

Biopsy or tissue material in a sterile container

1. Place biopsy material in a sterile container that can be sealed.
2. To prevent tissue from drying out, add several drops of sterile saline to keep moist if necessary.
3. Seal sterile container and place in a biohazard bag.

Swab in Amies transport medium

1. If swabs must be used, collect two swabs at the anatomic site of infection. One swab will be used for culture and one for Gram staining.
2. Place the swab in a tube of Amies transport medium.
3. Record on test requisition the anatomic site swabbed and suspected infection.



Storage & Transport

Temperature: Room temperature (15 °C – 25 °C / 59 °F – 77 °F)

Maximum Holding Time: 24 hours (time from collection to test set-up in laboratory)

2. Carba-R assay (rectal and perirectal swabs)



Specimen

Paired rectal swabs

1. The only swab that can be used is a Copan dual swab in Stuart medium.
2. Carefully insert both swab tips approximately 1 cm beyond the anal sphincter and rotate
3. See figure below for examples of acceptable swabs. Note, the swab cannot be overly contaminated with stool.

Paired perirectal swabs

1. The only swab that can be used is a Copan dual swab in Stuart medium.
2. Carefully insert both swab tips no more than 1 cm into the anal opening before the anal sphincter and rotate gently.
3. See figure below for examples of acceptable swabs. Note, the swab cannot be overly contaminated with stool.

Figure. Examples of Acceptable Swab Specimens for Xpert Carba-R Testing.



Storage & Transport

Temperature: Room temperature (15 °C – 28 °C / 59 °F – 82 °F)

Maximum Holding Time: 5 days (time from collection to test set-up in laboratory)

3. *Neisseria gonorrhoeae* culture

Specimen

Swab in Amies transport medium

1. Endocervical (preferred site for females)
 - a. Specimen collection should be done with a sterile Dacron swab.
 - b. Rotate swab against the wall of the endocervical canal several times for 20-30 seconds and withdraw without touching the vaginal surface.
 - c. Place the swab in a tube of Amies transport medium.
 - d. Speculum should be lubricated with water only.
2. Urethral (preferred site for males)
 - a. Delay obtaining specimen until 2 hours after patient has last voided.
 - b. Gently insert the urogenital swab into the urethra (women 1-2 cm, men 2-4 cm). Rotate the swab in one direction for at least one revolution for a minimum of 10 seconds.
 - c. Place the swab in a tube of Amies transport medium.
 - d. Alternatively, if a pus exudate can be expressed from the urethra to the tip of the penis, roll the swab in the exudate; place the swab in a tube of AMIES TRANSPORT MEDIUM.
3. Oropharynx (throat)
 - a. Swab the back of the throat and tonsillar area with a sterile swab.
 - b. Place the swab in a tube of Amies transport medium.
4. Rectal
 - a. Insert sterile swab approximately 1-1.5 inches in the anal canal. Move swab from side to side in the anal canal to sample crypts.
 - b. Allow swab to remain for 10-30 second for absorption of organisms onto the swab.
 - c. Place the swab in a tube of Amies transport medium.



Storage & Transport

Temperature: Room temperature (15 °C – 25 °C / 59 °F – 77 °F)

Maximum Holding Time: 24 hours (time from collection to test set-up in laboratory)

4. *Streptococcus* primary culture

Specimen

Throat swab

1. Depress tongue with a tongue depressor.
2. Sample the posterior pharynx, tonsils, and inflamed areas with a sterile swab.
3. Since many streptococcal species lose viability quickly, it is best to place swabs in an appropriate moist transport medium, such as Amies transport medium. If transport time is below 1 to 2 hours, a special transport system is not necessary.

Vaginal swab (for group B streptococcal screening)

1. Insert the swab 2 cm into the lower vagina (vaginal introitus).
2. Move the swab from side to side, or rotate the swab at each collection site, allowing 10 to 30 seconds for absorption of organisms into the swab material.
3. Place the swab in Amies transport medium.

Rectal swab (for group B streptococcal screening)

1. Insert sterile swab approximately 1-1.5 inches in the anal canal (through the anal sphincter). Move swab from side to side in the anal canal to sample crypts.
2. Allow swab to remain for 10 to 30 seconds for absorption of organisms into the swab material.
3. Place the swab in Amies transport medium.



Storage & Transport

Temperature: Room temperature (15–25 °C/59–77 °F)

Maximum Holding Time: 24 hours (time from collection to test set-up) for swabs in Amies transport medium

5. Stool culture

Specimen

Stool in Cary Blair medium

For the best results, stool specimens should be obtained during the acute phase of illness.

1. Lift the toilet seat and place the white stool collection device at the rear of the toilet bowl; lower the seat.
2. Pass the stool into the white stool collection device.
3. Collect stool from areas that appear bloody, slimy, or watery. If firm, collect from both ends and middle.
 - a. Using the scoop built into the cap, transfer enough stool to the vial to reach the red fill line, do not overfill.
 - b. Mix the vial contents with the scoop; carefully tighten the cap and shake until contents are well mixed.
 - c. Label the vial (name, collection date/time) and place inside the inner specimen bag and seal tightly.
4. Place the bagged yellow vial inside the zippered portion of the biohazard specimen bag and seal tightly.
5. Fill out the requisition form completely. Fold it in half once and place in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).
6. Transport at room temperature to the laboratory within 4 days of collection.



Stool collection device

Storage & Transport

Temperature: Room temperature (15–25 °C/59–77 °F) for Cary Blair Medium

Maximum Holding Time: 4 days (time from collection to test set-up) for Cary Blair Medium

6. Urine culture

Specimen

Urine in a Boritex Cup

1. Label the Boritex Cup with the patient's information.
2. Have the patient submit a clean-catch midstream urine sample in the Boritex Urine Cup (see additional instructions below).
3. Leave the white tablet in the cup. DO NOT INGEST. DO NOT TOUCH.
4. Place the Boritex Urine Culture Cup inside the biohazard specimen bag and seal tightly.
5. Fill out the requisition form completely. Fold it in half once (no staples please) and place in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).
6. Transport to the laboratory within 72 hours of collection.



Boritex Urine Culture Cup

Patient Instructions

Note: it is very important that these instructions are followed closely to prevent the urine sample from being contaminated with normal skin bacteria, which may result in the sample being rejected.

1. Ensure the Urine Collection Cup is labeled with your name and date of birth.
2. Wash your hands thoroughly with warm soapy water and dry well.
3. Spread a clean paper towel on a counter or surface you can reach from the toilet.
4. Open the towelette packets and place them on the towel.
5. Take the lid off the Urine Collection Cup. Put the lid (inside facing down) on the paper towel next to the towelettes. Do not touch the inside of the cup or lid.
6. Leave the white tablet in the cup. DO NOT INGEST. DO NOT TOUCH.
7. Cleanse the skin as follows:

Male Patients

- a. Wash your entire penis with the first wipe. Throw the towelette away.
- b. Pull back on the fold of skin around the tip of your penis (if present) and use the second towelette to cleanse the head of the penis from the center out. Throw the towelette away.
- c. Use the third towelette to cleanse the head of the penis from the center out; throw away.

Female Patients

1. Sit on the toilet and spread your legs apart. Use two fingers on one hand to spread open your labia (the folds of skin on each side of your vagina). Continue


- holding the labia open until you get the urine sample. The goal is to collect the urine directly into the container without coming in contact with surrounding skin.
2. With your other hand, use the first towelette to wipe the left side of the inner labial folds from front to back in one stroke. Throw the towelette away.
 3. Use the second towelette to wipe the right side of the inner labial folds from front to back in one stroke. Throw the towelette away.
 4. Use the third towelette to clean in the middle over the opening to your urethra. This is where your urine comes out, and it is just above the opening to your vagina. Throw the towelette away.
 8. Urinate the first part of the stream into the toilet and then stop the flow.
 9. Hold the urine collection cup a few inches from your urethra.
 10. Urinate into the cup until it is about half full and then stop the flow.
 11. Finish urinating in the toilet.
 12. Securely screw the lid onto the container, taking care not to touch the inside of the cup or lid. Rinse and dry the outside of the container.
 13. Wash your hands thoroughly with warm soapy water and dry.



Sterile Boritex Urine Collection Cup



Separate Labial Folds

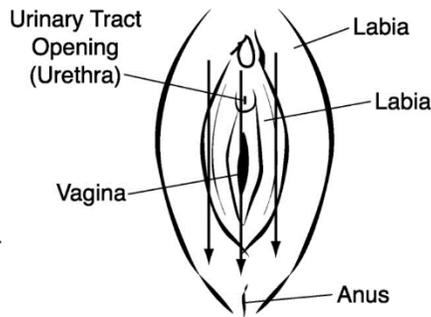

Wipe with Towlettes



Collect Urine

Storage & Transport

Temperature: Room temperature (15–25 °C/59–77 °F)

Maximum Holding Time: 72 hours (time from collection to test set-up).

Note: the Boritex Urine Culture Cup is the preferred specimen container and can be transported at room temperature within 72 hours. If the urine sample is submitted directly in a sterile container, it must be transported refrigerated and ASAP, but within 24 hours.

7. Urine: Legionella urinary antigen test

Specimen

Urine in a collection container

1. Urine specimen from a hospitalized patient collected in:
 - a. A sterile, leakproof container
 - b. A collection container with boric acid as a preservative (e.g., Boritex)
2. Specimen volume ≥ 5 mL

Storage & Transport

Temperature:

- Preferred: Refrigerated (2 to 8 °C / 36 to 46 °F)
- Accepted: Room temperature (15 to 30 °C / 59 to 86 °F) within 24 hours of collection
- Accepted: Frozen (-10 to -20 °C)

Maximum Holding Time:

- ≤ 14 days for refrigerated specimens
- ≤ 24 hours for specimens kept at room temperature
- ≤ 30 days for frozen specimens

c. Molecular test information

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Bordetella (pertussis) NAAT (2120)	Detection of <i>B. pertussis</i> and <i>B. parapertussis</i> DNA in respiratory specimens by Quidel Solana	NP swab	NP swab in VTM	Refrigerated (2–8°C): 72 hours	Negative	Daily	1 day	87798
Chlamydia NAAT (2750)	Qualitative detection of <i>Chlamydia trachomatis</i> ribosomal RNA by Hologic Panther	Urine, endocervical swab, rectal swab, throat swab, urethral swab, vaginal swab	<u>Urine</u> : Aptima urine container <u>Endocervical, urethral</u> : Aptima unisex swab <u>Rectal, throat, vaginal</u> : Aptima multitest swab	Room temp. or refrigerated (2–30°C): 30 days for urine, 60 days for swabs	Negative	Daily	1 day	87491
Enterovirus RT-PCR (6300)	Qualitative detection of Enterovirus RNA by RT-PCR	NP swab, throat swab, BAL, CSF, tracheal aspirate	<u>Swabs</u> : VTM <u>Others</u> : Sterile container	Refrigerated (2–8°C): 72 hours	Negative	Mon, Wed, Fri	2 days	87798
Gonorrhea NAAT (2770)	Qualitative detection of <i>Neisseria gonorrhoeae</i> ribosomal RNA by Hologic Panther	Urine, endocervical swab, rectal swab, throat swab, urethral swab, vaginal swab	<u>Urine</u> : Aptima urine container <u>Endocervical, urethral</u> : Aptima unisex swab <u>Rectal, throat, vaginal</u> : Aptima multitest swab	Room temp. or refrigerated (2–30°C): 30 days for urine, 60 days for swabs	Negative	Daily	1 day	87591

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Herpes Simplex Virus NAAT (6840)	Qualitative detection of HSV-1 and HSV-2 DNA by the Quidel Solana	Cutaneous and mucocutaneous lesions	Swab of lesion in VTM or UTM	Refrigerated (2–8°C): 7 days	Negative	Daily	1 day	87798
Influenza/SARS-CoV-2 NAAT (51000)	CDC Flu SC2 multiplex assay for qualitative detection of Influenza A, Influenza B, and SARS-CoV-2 RNA by PCR	<u>Swabs</u> : NP, throat, nasal mid-turbinate swab, anterior nasal <u>Other</u> : BAL, nasal wash/aspirate, pleural fluid, sputum, tracheal aspirate	<u>Swabs</u> : VTM <u>Fluids, aspirates</u> : Sterile container	Refrigerated (2–8°C): 72 hours Frozen (-70°C): >72 hours	Negative	Daily	1 day	87635
Influenza virus RT-PCR (51005)	CDC Human Influenza Virus RT-PCR Diagnostic Panel for Influenza A/B typing, subtyping, and lineage genotyping	<u>Swabs</u> : NP, throat, nasal mid-turbinate swab, anterior nasal <u>Other</u> : BAL, nasal wash/aspirate, pleural fluid, tracheal aspirate	<u>Swabs</u> : VTM <u>Fluids, aspirates</u> : Sterile container	Refrigerated (2–8°C): 72 hours Frozen (-70°C): >72 hours	Negative	Mon, Wed, Fri	1 day	87501
Mycoplasma genitalium NAAT (2870)	Qualitative detection of <i>Mycoplasma genitalium</i> ribosomal RNA by Hologic Panther	Urine, endocervical swab, urethral swab, vaginal swab	<u>Urine</u> : Aptima urine container <u>Endocervical, urethral</u> : Aptima unisex swab <u>Vaginal</u> : Aptima multitest swab	Room temp. or refrigerated (2–30°C): 30 days for urine, 60 days for swabs	Negative	3× weekly	2 days	87563

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Measles virus PCR (6180)	Qualitative detection of Measles virus RNA by RT-PCR	Throat swab, NP swab, NP aspirate, urine	<u>Swabs</u> : VTM <u>Urine, aspirates</u> : Sterile container	<u>Swabs, aspirates</u> : Refrigerated (2–8°C) for ≤72 hours; frozen (-70°C) for >72 hours <u>Urine</u> : Refrigerated (2–8°C) for ≤24 hours	Negative	Daily	1 day	87798
M. tuberculosis amplification, MTB-RIF (3530)	Qualitative detection of <i>Mycobacterium tuberculosis</i> complex DNA and rifampin resistance in respiratory specimens by Xpert MTB/RIF assay	Sputum, bronchial washings/aspirate	Sputum in a sterile container (≥5 ml); bronchial washings in a sterile container (≥1 ml)	Refrigerated (2–8°C): 72 hours	Negative	Daily	1 day	87556
Mumps Virus PCR (6170)	Qualitative detection of Mumps virus RNA by RT-PCR	<u>Tested inhouse</u> : Buccal swab <u>Referred</u> : Throat swab, urine	<u>Swabs</u> : VTM <u>Urine</u> : Sterile container	<u>Swabs</u> : Refrigerated (2–8°C) for ≤72 hours; frozen (-70°C) for >72 hours <u>Urine</u> : Refrigerated (2–8°C) for ≤24 hours	Negative	Daily	1 day	87798
Norovirus RT-PCR (6100)	Qualitative detection of Norovirus genogroup I and II RNA from stool specimens by PCR	Stool	Stool collected in Cary-Blair Medium or in a sterile container	<u>Cary-Blair</u> : room temperature (15–25°C) for up to 4 days <u>Raw stool</u> : Refrigerated (2–8°C) for up to 24 hours	Negative	Daily	1 day	87798

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Poxvirus PCR (BTC05300)	Qualitative detection of orthopoxvirus and non-variola orthopoxvirus DNA from lesions by PCR	Skin lesion	Dry swabs (x2) of a single lesion in a sterile container	Refrigerated (2–8°C): 7 days	Negative	Daily	1 day	87798
SARS-CoV-2/Flu/RSV NAAT (52000)	Multiplexed PCR for qualitative detection of RNA from SARS-CoV-2, influenza A, influenza B, and RSV by Xpert Xpress	NP swab, anterior nasal swab, nasal wash/aspirate	<u>Swabs and wash/aspirate</u> : VTM	Refrigerated (2–8°C): 7 days Room temp. (15–30°C): 2 days	Negative	Daily	1 day	87637, 87635
SARS-CoV-2 NAAT (6860)	Qualitative detection of SARS-CoV-2 RNA by transcription-mediated amplification by Hologic Panther	<u>Swabs</u> : NP, nasal, mid-turbinate, throat <u>Aspirate</u> : NP, nasal	<u>Swabs and aspirate</u> : VTM	Refrigerated (2–8°C): 72 hours	Negative	Daily	1 day	87635
Trichomonas NAAT (2850)	Qualitative detection of <i>Trichomonas vaginalis</i> ribosomal RNA by Hologic Panther	Urine, endocervical swab, vaginal swab	<u>Urine</u> : Aptima urine container <u>Endocervical</u> : Aptima unisex swab <u>Vaginal</u> : Aptima multitest swab	Room temp. or refrigerated (2–30°C): 30 days for urine, 60 days for swabs	Negative	3× weekly	2 days	87661

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Varicella-Zoster Virus NAAT (6900)	Qualitative detection of varicella-zoster virus (chickenpox) DNA by isothermal amplification with the Quidel Solana	Swabs of vesicular and non-vesicular lesions	<u>Swabs</u> : VTM	Refrigerated (2–8°C) or frozen (–20°C): 7 days	Negative	Daily	1 day	87798
Molecular panels								
Gastrointestinal PCR panel (6500)	Biofire PCR panel that detects 22 agents (viruses, bacteria, and parasites) that cause diarrhea	Stool	Stool in Cary-Blair transport medium (preferred), stool in a sterile container	<u>Cary-Blair</u> : ambient or refrigerated for up to 4 days <u>Sterile container</u> : ambient for 2 hours	No pathogens detected	Daily	1 day	0097U
Pneumonia PCR panel (6620)	Biofire PCR panel that detects 26 agents (viruses, bacteria, and atypical bacteria) that cause pneumonia, and 7 antimicrobial resistance genes	Sputum, BAL-like specimens	Sputum (≥1 ml) and BAL-like specimens (≥1 ml) in a sterile container	Refrigerated (2–8°C): 1 day	No pathogens detected	Daily	1 day	87798 (x 13), 87150 (x 7)

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Respiratory Pathogen PCR panel (6310)	Biofire PCR panel that detects 19 agents (viruses and bacteria) that cause respiratory illness	NP swab	NP swab in VTM	Refrigerated (2–8°C): 72 hours	No pathogens detected	Daily	1 day	0099U

BAL, bronchial alveolar lavage, NP, nasopharyngeal; PCR, polymerase chain reaction; RSV, respiratory syncytial virus; RT-PCR, reverse-transcription polymerase chain reaction; TAT, turnaround time (estimated maximum time from specimen receipt to result, where the time is dependent upon day of receipt, testing schedule, and length of testing); UTM, universal transport medium; VTM, viral transport medium.

d. Molecular specimen collection

1. Chlamydia, Gonorrhea, Trichomonas, and Mycoplasma genitalium NAAT testing

Specimen Type	Chlamydia	Gonorrhea	Trichomonas	M. genitalium
Urine (female/male)	✓	✓	✓	✓
Unisex Swab - Endocervical (female)	✓	✓	✓	✓
Unisex Swab - Urethral (male)	✓	✓		✓
Multitest Swab - Vaginal (female)	✓	✓	✓	✓
Multitest Swab - Throat (female/male)	✓	✓		
Multitest Swab - Rectal (female/male)	✓	✓		

Specimens

Urine – Urine transport tube

Patient Instructions

1. Do not urinate for at least one hour prior to collection.
2. Do not cleanse genitals prior to collection.
3. Collect only the first, most concentrated part of the urine stream (about 20 mL to 30 mL) into a collection cup that is free of any preservatives.



Clinic Staff Instructions

1. Using the disposable pipette provided, transfer 2 mL of urine into the transport tube, aiming for the middle of the fill area between the two black arrows.
 - a. If the volume is outside of the acceptable range indicated with black arrows, the specimen **will be rejected**. If urine is under the line, add more. If urine is over the line, discard and replace it with a new Aptima urine transport tube.
 - b. Urine specimens must be transferred into the transport tube within 24 hours of collection; however, we find within 2 hours to be optimal.
2. Tightly screw the cap onto the tube.

Endocervical swab – Unisex swab

1. Remove excess mucus from the cervical os and surrounding mucosa using the cleaning swab (white shaft swab). Discard this swab. If excess mucus remains, an additional large-tipped swab (not provided) may be used for cleaning.
2. Insert the Unisex Swab (blue shaft swab) into the endocervical canal.
3. Gently rotate the swab clockwise for 10 to 30 seconds in the endocervical canal.



Unisex Swab

4. Withdraw the swab carefully; avoid any contact with the vaginal mucosa.
5. Remove the tube cap and immediately place the swab into the transport tube.
6. Carefully break the swab shaft against the side of the tube at the scoreline and discard the top portion of the swab shaft; use care to avoid splashing of contents.
7. Re-cap the swab specimen transport tube tightly.

Urethral (Male) swab – Unisex swab

1. The patient should not have urinated for at least 1 hour prior to sample collection.
2. Insert the Unisex Swab (blue shaft swab) 2 to 4 cm into the urethra.
3. Gently rotate the swab clockwise for 2 to 3 seconds in the urethra; withdraw the swab carefully.
4. Remove the tube cap and immediately place the specimen collection swab into the transport tube.
5. Carefully break the swab shaft against the side of the tube at the scoreline and discard the top portion of the swab shaft; use care to avoid splashing of contents.
6. Re-cap the swab specimen transport tube tightly.



Unisex Swab

Vaginal swab – Multitest swab

Note: Vaginal swabs can be collected by the clinician or by the patient. Patient-collected vaginal swab specimens are an option for screening women when a pelvic exam is not otherwise indicated. The vaginal swab specimen collection kit is not for home use.

1. Partially peel open the swab package. Remove the swab. Do not touch the soft tip or lay the swab down. If the soft tip is touched, the swab is laid down, or the swab is dropped, use a new Aptima Multitest Swab Specimen Collection Kit.
2. Hold the swab, placing your thumb and forefinger in the middle of the swab shaft covering the score line. Do not hold the swab shaft below the score line.
3. Carefully insert the swab into the vagina about 2 inches (5 cm) and gently rotate the swab for 10 to 30 seconds. Make sure the swab touches the walls of the vagina so that moisture is absorbed by the swab and then withdraw the swab without touching the skin.
4. While holding the swab in the same hand, unscrew the cap from the tube. Do not spill the contents of the tube. If the contents of the tube are spilled, use a new Aptima Multitest Swab Specimen Collection Kit.
5. Immediately place the swab into the transport tube so that the score line is at the top of the tube.
6. Carefully break the swab shaft at the score line against the side of the tube.
7. Immediately discard the top portion of the swab shaft.
8. Tightly screw the cap onto the tube.



Multitest Swab

Throat swab – Multitest swab

1. Pull the swab out of the package. Do not touch the soft tip or lay the swab down.
2. Have patient tilt head back, breathe deeply, open mouth wide and say “Ah”. This serves to lift the uvula and aids in reducing the gag reflex.
3. Gently use tongue depressor to look for areas of inflammation (redness) and exudate (pus).
4. Carefully, but firmly, guide the Multitest Swab over:
 - a. Several areas of inflammation or pus
 - b. The tonsils (or tonsillar crypts if tonsils have been removed)
 - c. Posterior pharynx (back of throat)
5. Withdraw the swab carefully. Every effort should be made to avoid touching the swabs to the tongue, teeth, roof of the mouth or the inside of the cheeks at any time.
6. Remove the tube cap and immediately place the specimen collection swab into the transport tube.
7. Carefully break the swab shaft against the side of the tube at the scoreline and discard the top portion of the swab shaft; use care to avoid splashing of contents.
8. Re-cap the swab specimen transport tube tightly.



Multitest Swab

Rectal swab - Multitest swab

1. Pull the swab out of the package. Do not touch the soft tip or lay the swab down.
2. Insert the Aptima Multitest Swab approximately 3-5 cm into the rectum.
3. Gently rotate the swab clockwise for 2 to 3 seconds against the rectal wall; withdraw the swab carefully. Swabs that are grossly contaminated with feces should be discarded and the collection repeated.
4. Remove the tube cap and immediately place the specimen collection swab into the transport tube.
5. Carefully break the swab shaft against the side of the tube at the scoreline and discard the top portion of the swab shaft; use care to avoid splashing of contents.
6. Re-cap the swab specimen transport tube tightly.



Multitest Swab

Storage & Transport

Temperature: Refrigerated or room temperature (2 °C – 30 °C / 36 °F – 86 °F)


Maximum Holding Time: 30 days for urine; 60 days for swabs (time from collection to test set-up in lab)

2. Mumps PCR: Buccal swab

Specimen

Buccal swab in VTM

1. Collect a buccal swab sample as soon as mumps disease is suspected. RT-PCR has the greatest diagnostic sensitivity when samples are collected at first contact with a suspected case.
 - a. The buccal swab specimen is obtained by massaging the [parotid gland](#) area for 30 seconds prior to swabbing the area around Stensen's duct. A commercial product designed for the collection of throat specimens or a flocked polyester fiber swab can be used. Dacron or other synthetic swabs are required. Flocked synthetic swabs appear to be more absorbent and elute samples more efficiently.
 - i. Cotton swabs, or wood shafted swabs are unacceptable since they may contain substances that are inhibitory to enzymes used in RT-PCR.

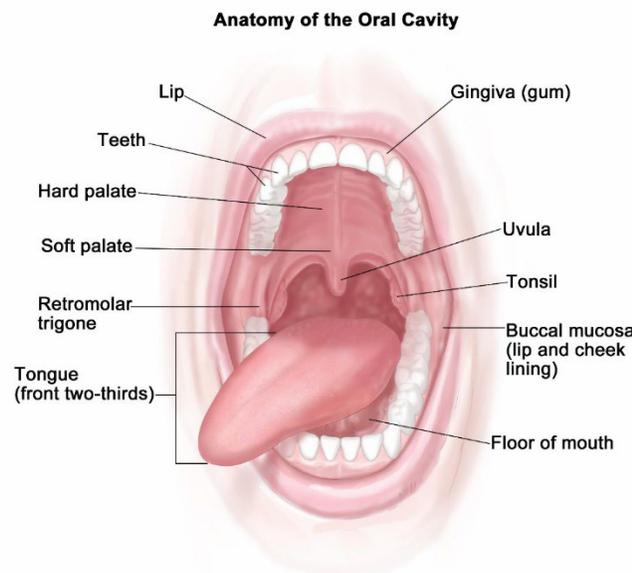

© 2012 Terese Winslow LLC
U.S. Govt. has certain rights

- b. Processing the swabs within 24 hours of collection will enhance the sensitivity of both the RT-PCR and virus isolation techniques.
- c. Swabs should be placed in 2 to 3 ml of standard viral transport medium (VTM). Swirl the swab VTM thoroughly and then ream the swab around the rim of the tube to retain cells and fluid in the tube. The swab can be broken off and left in the tube or discarded.

Collection Swabs & Viral Transport Media (VTM) tube



Storage & Transport

Temperature: Refrigerated temperature (2–8 °C/36–46 °F)

Maximum Holding Time: 24 hours refrigerated (time from collection to test set-up). If the specimen cannot be transported to the laboratory within 24 hours, freeze the specimen at the lowest temperature available. Frozen samples should be shipped on dry ice.

3. Poxvirus PCR: Lesion swab

Specimen

Lesion swab – dry swab in duplicate

1. Do not clean the lesion before sample collection. Also, do not apply a numbing cream or topical agent prior to swabbing as this may interfere with testing results.
2. Sample the skin lesions with a dry swab using a sterile nylon, polyester, or Dacron swab with a plastic or thin aluminum shaft. Do not use other types of swabs. Place in a sterile container and refrigerate within an hour of collection.
3. More than one lesion should be sampled, preferably 2 to 3 total lesions if present on different body sites. A lesion should be sampled with two separate swabs (second swab is confirmatory testing).
 1. **Vigorously** swab or brush the same lesion with two separate sterile dry swabs.
 2. Break off swabs and place each into separate sterile tubes or containers.
 3. Sample, label, and store each lesion separately. **Do not place in VTM or UTM.** Swabs must remain dry.
 4. Fill out the San Luis Obispo Public Health Laboratory Requisition completely.
 5. Indicate on requisition that you are requesting **Poxvirus testing**.
 6. Label the specimen with the patient's full name, date of collection, and specimen source.
 7. Include patient's vaccination history [date of smallpox (vaccinia) vaccination], clinical findings and symptoms (date of rash onset), and travel or exposure history on the requisition.

Storage & Transport

1. Refrigerate (2–8°C) dry swabs within an hour after collection. Transport at refrigerated temperature (wet ice) within 7 days. If specimens are to be held longer than 7 days, freeze (-20°C or lower) within an hour of collection and ship on dry ice.
2. Clinical specimens should be shipped in Category B packaging.

4. Respiratory testing: Bronchial alveolar lavage or tracheal aspirate

Specimen

Bronchial alveolar lavage or tracheal aspirate in a sterile container

1. Collect 2-3 mL into a sterile, leak-proof, screw-cap sputum collection cup or sterile dry container.
2. Due to the increased technical skill and equipment needs, collection of specimens other than sputum from the lower respiratory tract may be limited to patients presenting with more severe disease, including people admitted to the hospital and/or fatal cases.



Storage & Transport

Note: Storage and transport conditions depend on the type of testing performed. The most common conditions are described below. However, refer to the test information for exact conditions.

Temperature: Refrigerated (2–8 °C / 35.6–46.4 °F)

Maximum Holding Time: 72 hours (time from collection to test set-up in laboratory)

5. Respiratory testing: Nasopharyngeal aspirate

Specimen

Nasopharyngeal aspirate in VTM

1. Attach catheter to suction apparatus.
2. Tilt patient's head back 70 degrees.
3. Instill 1 mL-1.5 mL of non-bacteriostatic saline (pH 7.0) into one nostril.
4. Insert the tubing into the nostril parallel to the palate (not upwards). The catheter should reach a depth equal to distance from nostrils to outer opening of ear.
5. Begin gentle suction/aspiration and remove catheter while rotating it gently.
 - a. Place specimen in a collection container with 2–3 ml of VTM.

Storage & Transport

Note: Storage and transport conditions depend on the type of testing performed. The most common conditions are described below. However, refer to the test information for exact conditions.

Temperature: Refrigerated (2–8 °C / 35.6–46.4 °F)



Maximum Holding Time: 72 hours (time from collection to test set-up in laboratory)

6. Respiratory testing: Nasopharyngeal (NP) swab

Specimen

Nasopharyngeal swab

1. Collect respiratory specimen during acute phase of illness.
 - a. Ask the patient to blow their nose to clear their nasal passage and tilt the patient's head backwards.
 - b. Swiftly insert the small swab into one nostril straight back (not upwards) at a depth equal to distance from nostrils to outer opening of the ear (see image on backside of page).
 - c. Firmly rotate the swab up to 5 times and hold in place for 5-10 seconds to collect epithelial cells.
 - d. Repeat with the other nostril using the same swab.
2. Snap the swab at the scored breakpoint line; place swab into VTM tube; close the tube tightly.
3. Label the tube with the patient's name, date of birth, and the date/time of collection.
4. Place the collection tube inside the zippered portion of the biohazard specimen bag and seal tightly.
5. Fill out the requisition form completely. Fold it in half once (no staples please) and place the paperwork in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).

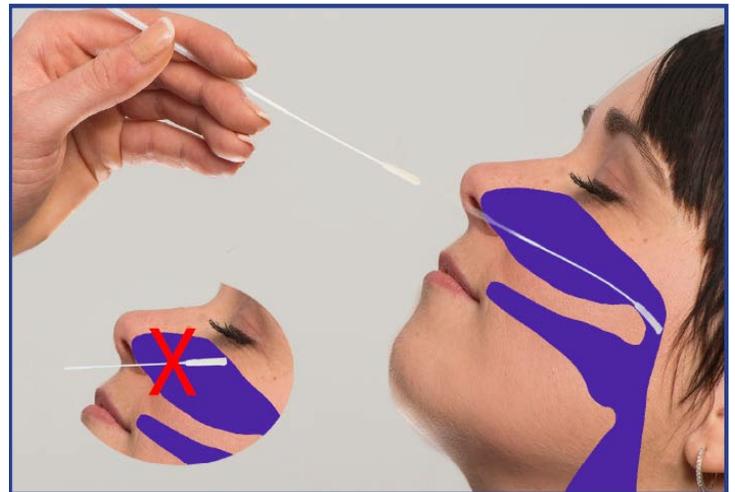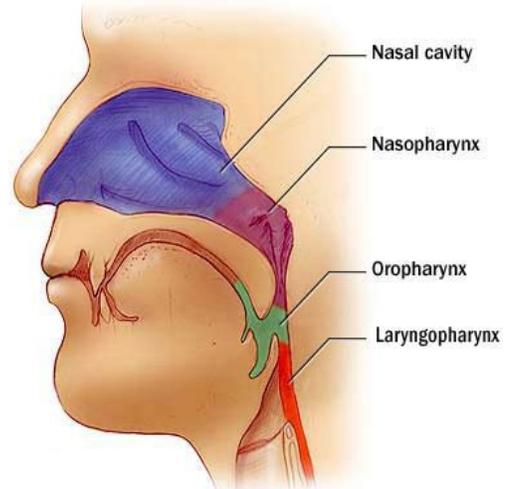

Storage & Transport

Temperature: Refrigerated (2–8 °C / 35.6–46.4 °F)

Maximum Holding Time: 72 hours (time from collection to test set-up in laboratory)

7. Respiratory specimen: throat swab

Specimen

Throat swab in VTM

1. Throat swabs should be taken with the aid of a tongue depressor.
2. Carefully insert swab into the posterior pharynx and tonsillar areas.
3. Rub swab over both tonsillar pillars and posterior oropharynx and avoid touching the buccal mucosa, tongue, teeth, and gums.
4. Place swab, tip first, into 2–3 ml of VTM.



Storage & Transport

Note: Storage and transport conditions depend on the type of testing performed. The most common conditions are described below. However, refer to the test information for exact conditions.

Temperature: Refrigerated (2–8 °C / 35.6–46.4 °F)

Maximum Holding Time: 72 hours (time from collection to test set-up in laboratory)

8. Stool collection: GP panel and norovirus testing

Specimen

Stool in Cary Blair medium

For the best results, stool specimens should be obtained during the acute phase of illness.

1. Lift the toilet seat and place the white stool collection device at the rear of the toilet bowl; lower the seat.
2. Pass the stool into the white stool collection device.
3. Collect stool from areas that appear bloody, slimy, or watery. If firm, collect from both ends and middle.
 - a. Using the scoop built into the cap, transfer enough stool to the vial to reach the red fill line, do not overfill.
 - b. Mix the vial contents with the scoop; carefully tighten the cap and shake until contents are well mixed.
 - c. Label the vial (name, collection date/time) and place inside the inner specimen bag and seal tightly.
4. Place the bagged yellow vial inside the zippered portion of the biohazard specimen bag and seal tightly.
5. Fill out the requisition form completely. Fold it in half once and place in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).
6. Transport at room temperature to the laboratory within 4 days of collection.



**Yellow vial of
Cary Blair Medium**



**Stool collection
device**

Storage & Transport

Temperature: Room temperature (15–25 °C/59–77 °F) for Cary Blair Medium

Maximum Holding Time: 4 days (time from collection to test set-up) for Cary Blair Medium

9. Stool collection: Norovirus testing

Specimen

Stool in sterile container

For the best results, stool specimens should be obtained during the acute phase of illness.

1. Label the sterile container (patient name, collection date/time).
2. Lift the toilet seat and place the white stool collection device at the rear of the toilet bowl; lower the seat.
3. Pass/expel the stool into the white stool collection device.
4. Using the wooden scoop, transfer stool from areas that appear bloody, slimy, or watery. If firm, collect from both ends and middle.
 - a. Transfer a walnut-sized amount of stool into the sterile container.
 - b. Place the scoop inside the sterile container.
 - c. Carefully tighten the cap.
 - d. Place the sterile container inside the zippered portion of the biohazard specimen bag and seal tightly.
5. Fill out the requisition form completely. Fold it in half once and place in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).
6. Transport at room temperature to the laboratory within 1 day of collection.



Sterile container



Stool collection device

Storage & Transport

Temperature: Refrigerated temperature (2–8 °C/36–46 °F) for stool in a sterile container

Maximum Holding Time: 1 day (time from collection to test set-up) for stool in a sterile container

10. Varicella zoster and Herpes: Lesion swabs

Specimen

Lesion swab in VTM

1. Optimal specimen collection time is within the first 3 days after appearance of the vesicular lesion. Prior to specimen collection, patients should avoid topical treatments as these may reduce virus yield.
2. Swab affected area:
 - a. Vesicular Lesion: Use a sterile needle to unroof the top of the vesicle. Use a sterile polyester swab to vigorously swab the base of the lesion, applying enough pressure to collect epithelial cells without causing bleeding while also collecting vesicular fluid. It is important to collect epithelial cells from the base of the lesion because they usually contain a significant amount of virus.
 - b. Non-Vesicular Lesion: Pre-moisten swab with saline. Collect cells from the base of the lesion.
3. Place swab into viral transport medium (VTM) or universal transport medium (UTM).
4. Place the collection tube inside the zippered portion of the biohazard specimen bag and seal tightly.
5. Fill out the requisition form completely. Fold it in half once (no staples please) and place in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).
6. Transport to the laboratory after collection. Specimen is stable at refrigerated temperatures for 7 days
6. Attach catheter to suction apparatus.

Storage & Transport

Temperature: Refrigerated (2°C–8°C/35.6°F–46.4°F) or Frozen (–20°C/–4°F)

Maximum Holding Time: 7 days (time from collection to test set-up in laboratory)

e. Mycobacteriology test information

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Acid fast bacilli concentration (9900)	Processing procedure to decontaminate and concentrate respiratory specimens	Sputum, bronchial wash, other non-sterile respiratory specimens	Respiratory specimen collected in a sterile container	Refrigerated (2–8°C): 3 days	N/A	Daily	1 day	87015
AFB culture (3545)	Culture and isolation of mycobacteria from primary specimens	Specimens from non-sterile sites (e.g., sputum) and sterile sites (e.g., CSF, joint fluid)	Specimens collected in a sterile container; tissue specimens may be kept moist with saline	Refrigerated (2–8°C): 3 days for most specimens, 24 hours for urine	Negative at 4 and 6 weeks	Daily	Prelim: 4 weeks if negative Final: 6 weeks if negative (longer if positive)	87116
AFB fluorescent smear (3535)	Auramine O stain (or equivalent) for fluorescent detection and visualization of acid-fast bacilli	Specimens from non-sterile sites (e.g., sputum) and sterile sites (e.g., CSF, joint fluid)	Specimens collected in a sterile container; tissue specimens may be kept moist with saline	Refrigerated (2–8°C): 3 days for most specimens, 24 hours for urine	No acid-fast bacilli seen	Daily	1 day	87206
AFB isolate identification, set-up (3555)	Culture procedure for suspect mycobacterial isolates	Mycobacterial isolate	AFB inoculated onto culture medium (slant preferred)	Room temp. (15–25°C): 7 days	No acid-fast bacilli present	Daily	2 weeks to ID or referral	87118

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
AFB tissue homogenization (3540)	Processing procedure to grind and homogenize tissue specimens	Tissue from various sites	Tissue collected in a sterile container, may be kept moist with sterile saline	Refrigerated (2–8°C): 3 days	N/A	Daily	1 day	87176
M. tuberculosis amplification, MTB-RIF (3530)	Qualitative detection of <i>Mycobacterium tuberculosis</i> complex DNA and rifampin resistance in respiratory specimens by Xpert MTB/RIF assay	Sputum, bronchial washings/aspirate	Sputum in a sterile container (≥5 ml); bronchial washings in a sterile container (≥1 ml)	Refrigerated (2–8°C): 72 hours	Negative	Daily	1 day	87556
MALDI-TOF MS mycobacterial ID (3660)	Mass spectrometry analysis to speciate mycobacteria isolates	Mycobacterial isolate	AFB on LJ Gruft, 7H11, or 7H11 select medium, or in MP broth	Culture conditions: 7 days for rapid growers; 2–4 weeks for slow growers	N/A	Weekly	2 weeks once isolated	87118
Quantiferon Plus (8800)	Whole blood assay for detection of active and latent tuberculosis	Whole blood	Collection into a set of 4 Quantiferon tubes	Room temp. (17–25°C): 16 hours	Negative	Wed	5 days	86480

AFB, acid-fast bacilli; LJ Gruft, Lowenstein Jensen Gruft; N/A, not applicable; TAT, turnaround time (estimated maximum time from specimen receipt to result, where the time is dependent upon day of receipt, testing schedule, and length of testing).

f. Mycobacteriology specimen collection

a. Sputum collection (mycobacteriology and mycology)

Specimen

Sputum


Sputum specimens should be collected in the early morning. Patients suspected of having TB should submit a minimum of 3 consecutive specimens at least 8 hours, but no more than 24 hours, apart.

1. Rinse throat and mouth with water (do not brush teeth or use mouthwash).
2. Cough very deeply and collect between 5 and 10 mL of sputum (about an inch high) into the specimen tube. Sputum is the mucus material from inside the lungs. Do not collect saliva or nasal discharge.
3. Tightly screw the cap onto the tube. If the cap is crooked, your specimen may leak and will be rejected.
4. Label the tube with the patient's name, date of birth, date collected and time collected.
5. Place the specimen tube inside the inner, clear specimen bag and seal the bag tightly.
6. Place the bagged specimen inside the zippered portion of the biohazard specimen bag and seal tightly.
7. Fill out the requisition form completely. Fold it in half once (no staples please) and place in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).
8. Transport to the laboratory within 72 hours of collection.

Storage & Transport

Temperature: Refrigerated (2 °C – 8 °C / 36 °F – 46 °F)

Maximum Holding Time: 72 hours (time from collection to test set-up in laboratory)

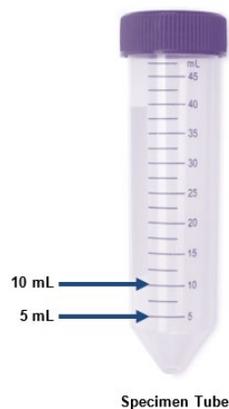

b. Cerebrospinal fluid

Specimen

Cerebrospinal fluid in a sterile container

2. CSF is obtained by lumbar puncture. During the procedure, a needle is typically inserted between the 3rd and 4th lumbar vertebrae and the CSF fluid is collected for testing.
3. A minimum of 2 ml should be collected and placed in a sterile container.

Storage & Transport

Note: Storage and transport conditions depend on the type of testing performed. The most common conditions are described below. However, refer to the test information for exact conditions.

Temperature: Refrigerated (2–8 °C / 35.6–46.4 °F)

Maximum Holding Time: 72 hours (time from collection to test set-up in laboratory)

3. Quantiferon Plus

Specimen

Blood in QuantiFERON Plus blood collection tubes



- a. **Fill blood tubes to correct volume:** The black mark on the side of the tubes indicates the 1 mL volume line. The QuantiFERON test has been validated for accuracy for tube volumes ranging from 0.8 to 1.2 mL. The 1 mL tubes fill slowly, so keep the tube on the needle for 2 - 3 seconds after the tube appears to have completed filling to ensure that the correct volume is drawn. If a “butterfly needle” is used, prime tubing with a “purge” tube before filling the QFT tubes to ensure proper fill volume.
- b. **Invert tubes 10 times:** Immediately after filling the tubes, invert them 10 times just firmly enough to ensure that the entire inner surface of the tube is coated with blood. Overly vigorous shaking may cause gel disruption and could lead to aberrant results. It is essential that the blood mixes thoroughly with the antigens that have been dried onto the inner wall of the tubes.
- c. **Label tubes:** Label each of the four tubes with the patient’s name & date of birth, as well as the collection date and time. Place the labeled collection tubes inside the zippered portion of the biohazard specimen bag and seal tightly.
- d. **Do not centrifuge, refrigerate, or freeze blood tubes.**
- e. **Complete requisition form:** Fold it in half once (no staples please) and place in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).
- f. **Transport at room temperature to the laboratory ASAP, but within 16 hours of collection.**

Storage & Transport

Temperature: room temperature (17 °C - 25 °C / 63 °F – 77 °F)

Maximum Holding Time: 16 hours, but ASAP preferred (Time from collection to test set-up in laboratory)

g. Mycology test information

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
MALDI-TOF MS mold ID (3950)	Mass spectrometry analysis to speciate mold (filamentous fungi) isolates	Mold isolate	Mold isolate on selective or non-selective agar (slant preferred)	Culture conditions: 48 hours	N/A	Weekly	1 week once isolated	87017
MALDI-TOF MS yeast ID (3950)	Mass spectrometry analysis to speciate yeast isolates	Yeast isolate	Yeast isolate on blood agar, Sabouraud-Dextrose agar, or Brain Heart Infusion agar	Culture conditions: 48 hours	N/A	Weekly	1 week once isolated	87016
Mycology culture: primary specimen (3905)	Culture and isolation of molds and yeast from primary specimens	Body fluid, scraping, or tissue	Varies (see mycology specimen collection instructions)	Varies (see mycology specimen collection instructions)	No growth at 1 week and 4 weeks	Daily	Prelim: 1 week Final: 4 weeks	87101
Mycology direct exam (3900)	KOH stain for detection of fungal elements in primary specimens	Body fluid, scraping, or tissue	Varies (see mycology specimen collection instructions)	Varies (see mycology specimen collection instructions)	No fungal elements seen	Daily	2 days	87220
Mycology identification, procedure (3980)	Biochemical, macroscopic, and/or microscopic analyses for identification of molds and yeast	Fungal isolate	Mold or yeast isolate on culture medium (slant preferred)	Room temp. (15-25°C): 7 days	N/A	Daily	2 weeks to ID or referral	87107

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Mycology isolate identification, set-up (3910)	Culture procedure for molds and yeast to set-up identification	Fungal isolate	Mold or yeast isolate on culture medium (slant preferred)	Room temp. (15-25°C): 7 days	N/A	Daily	2 weeks to ID or referral	87106

ID, identification; N/A, not applicable; TAT, turnaround time (estimated maximum time from specimen receipt to result, where the time is dependent upon day of receipt, testing schedule, and length of testing).

8. Mycology specimen collection

Specimen	Collection, storage, and transport
Abscess specimens	<ol style="list-style-type: none"> 1. Abscess material is aseptically aspirated in a clinical setting using a syringe. Transport syringe without a needle, or transfer material to a sterile screw-cap container. If the quantity is very small, 0.1 to 0.5ml of sterile saline may be added. 2. If specimen is collected surgically, also submit a portion of the abscess wall. 3. A non-cotton tip aerobic swab can be used, several, if possible, is optimal. Swabs for collection of material from draining fistulas and sinus tracts are the least preferred collection device. 4. Hold at 2–8°C, transport refrigerated or ambient within 72 hours, avoid freezing.
Body fluids other than CSF	<ol style="list-style-type: none"> 1. Bloody specimens should be collected in a heparinized syringe. 2. Non-bloody specimens are submitted in sterile containers. 3. A minimum of 1 ml should be collected. In general, the more fluid obtained for culture, the better the chance of isolation of any fungal pathogen. 4. Hold at 2–8°C, transport refrigerated or ambient within 72 hours, avoid freezing.
Bone marrow	<ol style="list-style-type: none"> A. Aseptically collect by sterile syringe or equivalent at least 0.3 ml to 1 ml in a sodium polyanethole sulfonate (SPS) or sodium heparin (heparin) blood tube. Transport to the lab within 24 hours, store at 2–8°C. Transport refrigerated or ambient, avoid freezing.
Bronchoalveolar lavage, transtracheal aspirate, bronchial brush	<ol style="list-style-type: none"> 1. Specimens are collected in a clinical setting; placed in a sterile container. 2. Bronchial brushes are placed in sterile saline, sterile distilled water, or brain heart infusion broth. 3. Hold specimen at 2–8°C. Transport to the laboratory refrigerated within 72 hours.
CSF	<ol style="list-style-type: none"> 1. CSF is obtained by lumbar puncture. A minimum of 2 ml should be collected and placed in a sterile container. 2. Hold at 2–8°C, transport refrigerated or ambient within 72 hours, avoid freezing.
Cultures for identification	<ol style="list-style-type: none"> 1. Submit a young, actively growing culture. Ideally isolates should be pure. 2. Cultures should be submitted immediately upon detection as some strains become pleomorphic over time making them difficult to identify.

Hair	<ol style="list-style-type: none"> 1. Collect 10 to 20 hairs, best detected using a Wood's Lamp. Place in a sterile dry container. If no fluorescence is observed, scrape scalp scales and pluck hairs at the edge of infection. 2. For Piedra, cut off several hairs with nodules attached. 3. Hold specimen at ambient or refrigerated temperature (2–8°C). Transport ambient or refrigerated; avoid freezing.
Nails	<ol style="list-style-type: none"> 1. Cleanse nail area with 70% alcohol and allow to air dry. Clip or scrape affected areas of nail deeply enough to obtain recently invaded nail tissue. Also, scrape the nail bed to collect debris under nail. Place specimen in a dry sterile container. Store and transport at ambient or refrigerated temperature (2–8°C).
Skin scrapings	<ol style="list-style-type: none"> 1. Cleanse area with 70% alcohol and allow to air dry. Scrape the lesion margin and place the material in a dry sterile container, be sure to collect any moist exudate. 2. Hold specimen at ambient or refrigerated temperature (2–8°C). Transport ambient or refrigerated; avoid freezing.
Sputum	<ol style="list-style-type: none"> a. Collect an early morning sputum produced by a deep cough into a sterile container. At least 5 ml of purulent material is optimal. Before collection the mouth should be cleansed; remove dentures or brush teeth. Induced sputum is acceptable. b. Deliver specimen to the laboratory as soon as possible, preferably within 2 hours of collection. If the specimen must be held, store at 2–8°C for up to 72 hours. Transport refrigerated. Never freeze the specimen. c. A fresh specimen is important because endogenous saprophytic organisms may overgrow the systemic pathogens or inhibit them by acidifying the culture media.
Tissue and biopsy specimens	<ol style="list-style-type: none"> 1. Generally, tissue and biopsy specimens are collected in a clinical setting and placed in a sterile screw-cap container with a small amount of sterile saline to prevent drying. 2. Hold at 2–8°C. Transport specimen refrigerated or ambient within 72 hours. Avoid freezing.
Urine	<ol style="list-style-type: none"> 1. Collect 10 to 50 ml of clean-catch urine (first morning is best), catheterized urine, or suprapubic aspirate in a sterile screw cap cup. Store the specimen at 2–8°C. Transport to the laboratory refrigerated within 72 hours. Avoid freezing. 2. Urine preservative collection systems can be used for urinary tract infection culture but are not acceptable for systemic pathogen culture. Follow the manufacturer's transport and

	holding instructions for individual preservative systems.
--	---

i. Parasitology test information

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
<i>Cyclospora</i> direct exam (4045)	Processing, staining, and examination of stool for <i>Cyclospora</i> oocysts	Stool	Stool in O&P vials (preferred) or a sterile container	<u>O&P vials</u> : Room temp. (15–25°C) for 7 days <u>Sterile container</u> : Room temp. (15–25°C) for 24 hours	Negative	Daily	2 days	87206, 87015
Helminth-Arthropod identification (4020)	Direct examination of arthropod material to identify tick genus	Intact helminth or arthropod	Container without denaturing substances (e.g., 70% alcohol)	Room temp. (15–25°C) or refrigerated (2–8°C): 7 days	No helminth or arthropod found	Daily	1 day	87169
<i>Isospora</i> special direct exam (4065)	Processing, staining, and examination of stool for <i>Isospora</i> oocysts	Stool	Stool in O&P vials (preferred) or a sterile container	<u>O&P vials</u> : Room temp. (15–25°C) for 7 days <u>Sterile container</u> : Room temp. (15–25°C) for 24 hours	Negative	Daily	2 days	87206, 87015
<i>Microsporidia</i> special direct exam (4060)	Processing, staining, and examination of stool for <i>Microsporidia</i> spores	Stool	Stool in O&P vials (preferred) or a sterile container	<u>O&P vials</u> : Room temp. (15–25°C) for 7 days <u>Sterile container</u> : Room temp. (15–25°C) for 24 hours	No <i>Microsporidia</i> seen	Daily	2 days	87206, 87015
Ova and parasites, concentration, and exam (4025)	Processing and wet mount examination of stool for ova and worms	Stool	Stool in O&P vials (preferred) or a sterile container	<u>O&P vials</u> : Room temp. (15–25°C) for 7 days <u>Sterile container</u> : Room temp. (15–25°C) for 24 hours	No ova or parasites seen	Daily	3 days	87177

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Parasite blood smear exam (4040)	Preparation and examination of thick and thin blood smears for parasites	Blood or prepared thick and thin smears (×4)	Whole blood collected in EDTA	Room temp. (15–25°C): 1 day	Negative	Daily	1 day	86750
Parasite identification—Trichrome stain (4010)	Processing, staining, and examination of stool for intestinal protozoa	Stool	Stool in O&P vials (preferred) or a sterile container	<u>O&P vials</u> : Room temp. (15–25°C) for 7 days <u>Sterile container</u> : Room temp. (15–25°C) for 24 hours	No protozoa seen	Daily	3 days	87209
Parasite special direct exam (4000)	Macroscopic and microscopic examination of specimen for parasites, primarily worms	Suspected parasite material	Container without denaturing substances (e.g., 70% alcohol)	Room temp. (15–25°C): 1 day Refrigerated (2–8°C): 3 days or before desiccation	No parasites seen	Daily	2 days	87207
Pinworm prep (4005)	Microscopic examination of paddles for pinworm eggs and adult worms	Sample from skin around the anal opening	Pinworm paddle is used to sample skin around the anal opening	Room temp. (15–25°C): 1 day Refrigerated (2–8°C): 7 days	Negative	Daily	1 day	87172

O&P, ova & parasite; TAT, turnaround time (estimated maximum time from specimen receipt to result, where the time is dependent upon day of receipt, testing schedule, and length of testing).

j. Parasitology specimen collection

1. Blood smear for parasites

Specimen

EDTA blood tube

1. Collect an EDTA tube with the draw time marked on the tube as well as the date and patient's name.
2. Make a minimum of four (4) thick and four (4) thin smears as soon as possible or WITHIN 4 HOURS OF COLLECTION. DO NOT FIX.
 - a. Note: Thick and thin smears can also be prepared at the laboratory.

Storage & Transport

1. Store EDTA tube and blood smears at room temperature (15–25 °C/59–77 °F).
2. Optimally, the EDTA tube and smears should be delivered to the laboratory on the same day as collection.

2. Pinworm collection

Specimen

Sampling of anal area with a pinworm paddle

1. Specimens are best collected first thing in the morning before bathing and before a bowel movement. Collect one specimen each morning for 4 to 6 consecutive days.
2. Remove one specimen tube from the package.
3. Expose the anal area by gently separating the cheeks. Do not insert the paddle into the rectum.
4. Press the sticky side of the paddle against the skin on several areas around the anal opening.
5. Insert the paddle back into the tube and press firmly to close. Label outside tube with patient name, date of birth, and collection date and time.
6. Place the specimen tube inside the zippered portion of the biohazard specimen bag and seal tightly.
7. Collect 3 to 5 more specimens on consecutive mornings and place those inside the biohazard bag as well.
8. Fill out the requisition form(s) completely. Place in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).



Storage & Transport

Temperature: room temperature (15–25 °C / 59-77 °F) for the first 24 hours and refrigerated (2-8 °C / 35-46 °F) for up to 7 days

Maximum Holding Time: 7 days

3. Stool collection: Ova and parasites

Specimen

Stool in O&P vial

Preferably, three stool specimens should be collected (one every other day) as soon as symptoms develop.

1. Lift the toilet seat and place the white stool collection device at the rear of the toilet bowl; lower the seat.
2. Pass the stool into the white stool collection device.
3. Collect stool from areas that appear bloody, slimy, or watery. If firm, collect from both ends and middle.
 - a. Using the scoop built into the cap, transfer enough stool to each vial to reach the red fill line.
 - b. Mix the vial contents with the scoop; carefully tighten the cap and shake until contents are well mixed.
 - c. Label the vials (name, collection date/time) and place inside the inner specimen bag and seal tightly.
4. Place the bagged vials inside the zippered portion of the biohazard specimen bag and seal tightly.

5. Fill out the requisition form completely. Fold it in half once (no staples please) and place in the outer pocket of the biohazard specimen bag (not inside the zippered pouch with the specimen).
6. Transport to the laboratory within 7 days of collection.



stool collection device



O&P Collection Kit

*Warning: vial contents are poisonous.
Keep out of reach of children.*

Storage & Transport

Temperature: Room temperature (15 °C – 25 °C / 59 °F – 77 °F)

Maximum Holding Time: 7 days (time from collection to test set-up in laboratory)

k. Serology test information

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Blood lead (9150)	Determination of the concentration of lead in a capillary blood sample	Blood (fingerstick)	Blood from a fingerstick is collected in capillary tube and transferred into Treatment Reagent	Room temp. (15–25°C): 2 days Refrigerated (2–8°C): 7 days	<3.3 ug/dL	Daily	1 day	83655
HIV antigen & antibody immunoassay, serum (5500)	Qualitative detection of HIV p24 antigen, antibodies to HIV-1, and antibodies to HIV-2 in blood	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, heparin, or plasma-separator tube	Refrigerated (2–8°C): 7 days	Non-reactive	Tue, Thu	3 days	87389
HIV antibody differentiation test (5700)	Confirmation and differentiation of antibodies to HIV-1 and HIV-2 in blood	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, or heparin tube	Room temp. (18–30°C): 2 days Refrigerated (2–8°C): 7 days	Negative	Day after screen	4 days	86703
RPR, serum (5035)	Detection of anti-lipid antibodies (reagin) in serum or plasma	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, heparin, or CPD tube	<u>Serum</u> : Refrigerated (2–8°C) for 5 days; frozen (<-20°C) for 30 days <u>Plasma</u> : Refrigerated (2–8°C) for 48 hours	Non-reactive	Mon, Tue, Thu	2 days	86592

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
RPR, serum, titer (5040)	Titer determination of anti-lipid antibodies (reagin) in serum or plasma	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, heparin, or CPD tube	<u>Serum</u> : Refrigerated (2–8°C) for 5 days; frozen (<-20°C) for 30 days <u>Plasma</u> : Refrigerated (2–8°C) for 48 hours	Non-reactive	Mon, Tue, Thu	2 days	86593
<i>Treponema pallidum</i> particle agglutination test (5065)	Qualitative detection of antibodies against <i>Treponema pallidum</i> in serum or plasma	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, or heparin tube	<u>Serum</u> : Refrigerated (2–8°C) for 5 days; frozen (<-20°C) for 30 days <u>Plasma</u> : Refrigerated (2–8°C) for 48 hours	Non-reactive	Mon, Tue, Thu	3 days	86780
Varicella-Zoster (VZV) antibody (5100)	Qualitative detection of human IgG antibodies to varicella zoster virus in serum	Serum	Venous blood collected in serum or serum-separator tube	Refrigerated (2–8°C): 48 hours Frozen (<-20°C): for 30 days	Positive	Mon	5 days	86787
VDRL, CSF (5060)	Qualitative detection of anti-lipid antibodies (reagin) in CSF	CSF	CSF collected in a sterile container	Refrigerated (2–8°C): 5 days	Non-reactive	Tue, Thu	3 days	86592
VDRL, CSF, titer (5050)	Quantitative detection of anti-lipid antibodies (reagin) in CSF	CSF	CSF collected in a sterile container	Refrigerated (2–8°C): 5 days	Non-reactive	Tue, Thu	3 days	86593

CPD, citrate phosphate dextrose; CSF, cerebrospinal fluid; TAT, turnaround time (estimated maximum time from specimen receipt to result, where the time is dependent upon day of receipt, testing schedule, and length of testing).

I. Serology specimen collection

1. Blood lead testing

Specimen

LeadCare II Capillary Tube

Note: Only use the heparinized Capillary Tubes provided with the LeadCare II Test Kit. The Capillary Tube must be filled to the fill line (50µl) for accurate results. Check to make sure that the tube is free of gaps and bubbles. After collection, wipe the Capillary Tube with gauze pad (wipe downward). The accuracy of the test depends on the precisely measured sample.

1. Place all collection materials on top of disposable pad. Label a Treatment Reagent tube with the patient ID using the label provided. Open the lancet, alcohol swabs, gauze, bandage, and other items. Have all items ready for blood collection.
2. Wash hands with soap. Do not use recycled disposable paper towels. Allow to air dry. Do not allow child's finger to touch any surface. Put on your powder-free gloves.
3. Remove a Capillary Tube and Plunger from container and place on top of lid of container to have ready for use.
4. Remove the Treatment Reagent cap from the labeled tube and place it top down on pad. Do not allow the inside of the cap to touch anything. This could contaminate the sample.
5. Massage the patient's hand and lower part of the finger to increase blood flow. Turn the hand down.
6. Scrub the patient's middle finger or ring finger with an alcohol swab and allow to air dry.
7. Hold the finger in a downward position and lance the palm side surface of the finger.
8. Apply slight pressure to start blood flow. Blot the first drop of blood on a gauze pad and discard in appropriate container.
9. Keep the finger in a downward position to maintain blood flow. Hold the Capillary Tube at an angle of 10 degrees below the collection site and touch the tapered end of the tube into the droplet of blood. Do not touch the skin with the tube. Fill to the 50 µL black line. Filling stops when the sample reaches the black line.
10. Remove excess blood from the outside of the tube with a clean wipe or gauze pad. Use a downward motion to wipe excess blood from the capillary tube. Use caution not to absorb the blood from the end of the Capillary Tube.
11. Inspect the Capillary Tube for proper filling. Make sure there are no gaps, air bubbles, or any excess blood on the outside of the Capillary Tube.
12. Place the full Capillary Tube in the Treatment Reagent. Insert Plunger into the top of the Capillary Tube and push down, ensuring to dispense the entire volume into the Treatment Reagent within 10 minutes.
13. Replace the tube cap. Invert the tube 8 to 10 times to mix the sample completely.
14. The test sample is ready when the mixture turns brown.

15. Once the sample is collected, apply slight pressure to the finger to stop the bleeding. Apply a sterile adhesive bandage over the puncture site.

Storage & Transport

- a. The mixture of blood and Treatment Reagent is stable for up to 48 hours at room temperature and up to 7 days refrigerated.

b. Serum

Specimen

Serum in a serum separator tube (SST)

1. Collect ≥ 5 ml of blood into an SST by venipuncture.
2. If possible, centrifuge the blood immediately afterward.

Storage & Transport

Note: Storage and transport conditions depend on the type of testing performed. The most common conditions are described below. However, refer to the test information for exact conditions.



Non-centrifuged blood

Temperature: Room temperature (15–25 °C/59–77 °F)

Maximum Holding Time: 24 hours (time from collection to receipt by laboratory)

Centrifuged blood

Temperature: Refrigerated (2–8 °C / 35.6–46.4 °F)

Maximum Holding Time: 7 days (time from collection to test set-up in laboratory)

m. Sexually-transmitted infection test information

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Chlamydia NAAT (2750)	Qualitative detection of <i>Chlamydia trachomatis</i> ribosomal RNA by Hologic Panther	Urine, endocervical swab, rectal swab, throat swab, urethral swab, vaginal swab	<u>Urine</u> : Aptima urine container <u>Endocervical, urethral</u> : Aptima unisex swab <u>Rectal, throat, vaginal</u> : Aptima multitest swab	Room temp. or refrigerated (2–30°C): 30 days for urine, 60 days for swabs	Negative	Daily	1 day	87491
Gonorrhea NAAT (2770)	Qualitative detection of <i>Neisseria gonorrhoeae</i> ribosomal RNA by Hologic Panther	Urine, endocervical swab, rectal swab, throat swab, urethral swab, vaginal swab	<u>Urine</u> : Aptima urine container <u>Endocervical, urethral</u> : Aptima unisex swab <u>Rectal, throat, vaginal</u> : Aptima multitest swab	Room temp. or refrigerated (2–30°C): 30 days for urine, 60 days for swabs	Negative	Daily	1 day	87591
Herpes Simplex Virus NAAT (6840)	Qualitative detection of HSV-1 and HSV-2 DNA by the Quidel Solana	Cutaneous and mucocutaneous lesions	Swab of lesion in VTM or UTM	Refrigerated (2–8°C): 7 days	Negative	Daily	1 day	87798
HIV antigen & antibody immunoassay, serum (5500)	Qualitative detection of HIV p24 antigen, antibodies to HIV-1, and antibodies to HIV-2 in blood	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, heparin, or plasma-separator tube	Refrigerated (2–8°C): 7 days	Non-reactive	Tue, Thu	3 days	87389

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
HIV antibody differentiation test (5700)	Confirmation and differentiation of antibodies to HIV-1 and HIV-2 in blood	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, or heparin tube	Room temp. (18–30°C): 2 days Refrigerated (2–8°C): 7 days	Negative	Day after screen	4 days	86703
Mycoplasma genitalium NAAT (2870)	Qualitative detection of <i>Mycoplasma genitalium</i> ribosomal RNA by Hologic Panther	Urine, endocervical swab, urethral swab, vaginal swab	<u>Urine</u> : Aptima urine container <u>Endocervical</u> , <u>urethral</u> : Aptima unisex swab <u>Vaginal</u> : Aptima multitest swab	Room temp. or refrigerated (2–30°C): 30 days for urine, 60 days for swabs	Negative	3× weekly	2 days	87563
Neisseria gonorrhoeae culture (2050)	Culture and isolation of <i>Neisseria gonorrhoeae</i> from primary specimens	Swab of urogenital, cervical, rectal, or oropharyngeal site	Dacron or rayon swab of site placed in Amies transport medium	Ambient for up to 48 hours	No pathogen isolated	Daily	3 days	87850
RPR, serum (5035)	Detection of anti-lipid antibodies (reagin) in serum or plasma	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, heparin, or CPD tube	<u>Serum</u> : Refrigerated (2–8°C) for 5 days; frozen (<-20°C) for 30 days <u>Plasma</u> : Refrigerated (2–8°C) for 48 hours	Non-reactive	Mon, Tue, Thu	2 days	86592

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
RPR, serum, titer (5040)	Titer determination of anti-lipid antibodies (reagin) in serum or plasma	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, heparin, or CPD tube	<u>Serum</u> : Refrigerated (2–8°C) for 5 days; frozen (<-20°C) for 30 days <u>Plasma</u> : Refrigerated (2–8°C) for 48 hours	Non-reactive	Mon, Tue, Thu	2 days	86593
<i>Treponema pallidum</i> particle agglutination test (5065)	Qualitative detection of antibodies against <i>Treponema pallidum</i> in serum or plasma	Serum (preferred) or plasma	Venous blood collected in serum, serum-separator, EDTA, sodium citrate, or heparin tube	<u>Serum</u> : Refrigerated (2–8°C) for 5 days; frozen (<-20°C) for 30 days <u>Plasma</u> : Refrigerated (2–8°C) for 48 hours	Non-reactive	Mon, Tue, Thu	3 days	86780
Trichomonas NAAT (2850)	Qualitative detection of <i>Trichomonas vaginalis</i> ribosomal RNA by Hologic Panther	Urine, endocervical swab, vaginal swab	<u>Urine</u> : Aptima urine container <u>Endocervical</u> : Aptima unisex swab <u>Vaginal</u> : Aptima multitest swab	Room temp. or refrigerated (2–30°C): 30 days for urine, 60 days for swabs	Negative	3× weekly	2 days	87661
VDRL, CSF (5060)	Qualitative detection of anti-lipid antibodies (reagin) in CSF	CSF	CSF collected in a sterile container	Refrigerated (2–8°C): 5 days	Non-reactive	Tue, Thu	3 days	86592

CPD, citrate phosphate dextrose; CSF, cerebrospinal fluid; TAT, turnaround time (estimated maximum time from specimen receipt to result, where the time is dependent upon day of receipt, testing schedule, and length of testing).

n. Sexually-transmitted infection specimen collection

Refer to specimen collection instructions for molecular testing, mycobacteriology, and serology.

o. Virology test information

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Herpes Simplex Virus NAAT (6840)	Qualitative detection of HSV-1 and HSV-2 DNA by the Quidel Solana	Cutaneous and mucocutaneous lesions	Swab of lesion in VTM or UTM	Refrigerated (2–8°C): 7 days	Negative	Daily	1 day	87798
Influenza virus RT-PCR (51005)	CDC Human Influenza Virus RT-PCR Diagnostic Panel for Influenza A/B typing, subtyping, and lineage genotyping	<u>Swabs</u> : NP, throat, nasal mid-turbinate swab, anterior nasal <u>Other</u> : BAL, nasal wash/aspirate, pleural fluid, tracheal aspirate	<u>Swabs</u> : VTM <u>Fluids, aspirates</u> : Sterile container	Refrigerated (2–8°C): 72 hours Frozen (-70°C): >72 hours	Negative	Mon, Wed, Fri	1 day	87501
Measles virus PCR (6180)	Qualitative detection of Measles virus RNA by RT-PCR	Throat swab, NP swab, NP aspirate, urine	<u>Swabs</u> : VTM <u>Urine, aspirates</u> : Sterile container	<u>Swabs, aspirates</u> : Refrigerated (2–8°C) for ≤72 hours; frozen (-70°C) for >72 hours <u>Urine</u> : Refrigerated (2–8°C) for ≤24 hours	Negative	Daily	1 day	87798
Mumps Virus PCR (6170)	Qualitative detection of Mumps virus RNA by RT-PCR	<u>Tested inhouse</u> : Buccal swab <u>Referred</u> : Throat swab, urine	<u>Swabs</u> : VTM <u>Urine</u> : Sterile container	<u>Swabs</u> : Refrigerated (2–8°C) for ≤72 hours; frozen (-70°C) for >72 hours <u>Urine</u> : Refrigerated (2–8°C) for ≤24 hours	Negative	Daily	1 day	87798

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Norovirus RT-PCR (6100)	Qualitative detection of Norovirus genogroup I and II RNA from stool specimens by PCR	Stool	Stool collected in Cary-Blair Medium or in a sterile container	<u>Cary-Blair</u> : room temperature (15–25°C) for up to 4 days <u>Raw stool</u> : Refrigerated (2–8°C) for up to 24 hours	Negative	Daily	1 day	87798
Rabies DFA (6000)	Detection of rabies virus in brain tissue using a direct fluorescent antibody technique	Brain tissue	Intact head, complete carcass, or brain from a suspect rabid animal	Refrigerated (2–8°C): 72 hours	Negative	Daily	1 day	N/A
SARS-CoV-2 NAAT (6860)	Qualitative detection of SARS-CoV-2 RNA by transcription-mediated amplification by Hologic Panther	<u>Swabs</u> : NP, nasal, mid-turbinate, throat <u>Aspirate</u> : NP, nasal	<u>Swabs and aspirate</u> : VTM	Refrigerated (2–8°C): 72 hours	Negative	Daily	1 day	87635
Varicella-Zoster Virus NAAT (6900)	Qualitative detection of varicella-zoster virus (chickenpox) DNA by isothermal amplification with the Quidel Solana	Swabs of vesicular and non-vesicular lesions	<u>Swabs</u> : VTM	Refrigerated (2–8°C) or frozen (–20°C): 7 days	Negative	Daily	1 day	87798

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Varicella-Zoster (VZV) antibody (5100)	Qualitative detection of human IgG antibodies to varicella zoster virus in serum	Serum	Venous blood collected in serum or serum-separator tube	Refrigerated (2–8°C): 48 hours Frozen (<-20°C): for 30 days	Positive	Mon	5 days	86787
Virology panels								
Gastrointestinal PCR panel (6500)	Biofire PCR panel that detects 22 agents (viruses, bacteria, and parasites) that cause diarrhea	Stool	Stool in Cary-Blair transport medium (preferred), stool in a sterile container,	<u>Cary-Blair</u> : ambient or refrigerated for up to 4 days <u>Sterile container</u> : ambient for 2 hours	No pathogens detected	Daily	1 day	0097U
Influenza/SARS-CoV-2 NAAT (51000)	CDC Flu SC2 multiplex assay for qualitative detection of Influenza A, Influenza B, and SARS-CoV-2 RNA by PCR	<u>Swabs</u> : NP, throat, nasal mid-turbinate swab, anterior nasal <u>Other</u> : BAL, nasal wash/aspirate, pleural fluid, sputum, tracheal aspirate	<u>Swabs</u> : VTM <u>Fluids, aspirates</u> : Sterile container	Refrigerated (2–8°C): 72 hours Frozen (-70°C): >72 hours	Negative	Daily	1 day	87635
Pneumonia PCR panel (6620)	Biofire PCR panel that detects 26 agents (viruses, bacteria, and atypical bacteria) that cause pneumonia, and 7 antimicrobial resistance genes	Sputum, BAL-like specimens	Sputum (≥1 ml) and BAL-like specimens (≥1 ml) in a sterile container	Refrigerated (2–8°C): 1 day	No pathogens detected	Daily	1 day	87798 (x 13), 87150 (x 7)

Test (Order code)	Description	Specimen(s)	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)	CPT code
Respiratory Pathogen PCR panel (6310)	Biofire PCR panel that detects 19 agents (viruses and bacteria) that cause respiratory illness	NP swab	NP swab in VTM	Refrigerated (2-8°C): 72 hours	No pathogens detected	Daily	1 day	0099U
SARS-CoV-2/Flu/RSV NAAT (52000)	Multiplexed PCR for qualitative detection of RNA from SARS-CoV-2, influenza A, influenza B, and RSV by Xpert Xpress	NP swab, anterior nasal swab, nasal wash/aspirate	<u>Swabs and wash/aspirate:</u> VTM	Refrigerated (2-8°C): 7 days Room temp. (15-30°C): 2 days	Negative	Daily	1 day	87637, 87635

N/A, not applicable; RT-PCR, reverse transcriptase-polymerase chain reaction; TAT, turnaround time (estimated maximum time from specimen receipt to result, where the time is dependent upon day of receipt, testing schedule, and length of testing); UTM, universal transport medium; VTM, viral transport medium.

p. Virology specimen collection

Refer to specimen collection instructions for molecular and serology.

1. Animals for rabies testing

Specimens

Whole animal (if no larger than a racoon)

- i. Triple bag the whole animal, securing each bag individually with tape or equivalent.
- ii. Place the completed requisition in a separate plastic bag—do not place the requisition in the bag containing the animal carcass.
- iii. Refrigerate the specimens (no more than 3 days); transport them to the public health laboratory as soon as possible.

Animal head (for larger animals)

1. When removing the head be aware that the spinal cord near the base of the head is an important section for testing rabies.
2. For large heads triple bag as for whole animals.
3. For small heads or small animals (i.e., bats) place the head or carcass in a plastic or Ziplock bag, and then place in a secondary plastic bag and then in a third plastic bag.
4. Refrigerate the specimens (no more than 3 days); transport them to the public health laboratory as soon as possible.
5. DO NOT FREEZE THE ANIMAL.

Transport

1. Place bagged animal in a cooler or Styrofoam container with several ice packs for transport.
2. Place filled out requisition in a yellow leak-proof Biohazard bag and put it in the cooler for transport.
3. If there is more than one animal of the same species be sure to provide distinct identification for each one separately on separate requisitions.

q. Water and shellfish test information

Test (Order code)	Description	Sample	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)
Drinking water							
Total coliforms & <i>E. coli</i> Presence-Absence (8040)	Detection of total coliforms and <i>E. coli</i> in potable drinking water	Drinking water	Collection in a 100 mL Idexx bottle	Refrigerated (2–8°C): 30 hours	Absent	Daily	1 day
Total coliforms & <i>E. coli</i> MPN, Undiluted (8350)	Detection and enumeration of total coliforms and <i>E. coli</i> in potable drinking water	Drinking water	Collection in a 100 mL Idexx bottle	Refrigerated (2–8°C): 30 hours	<1 MPN/100 mL	Daily	1 day
Heterotrophic plate count (8045)	Estimation of the number of live heterotrophic bacteria in a water sample	Drinking water	Collection in a 100 mL Idexx bottle	Refrigerated (2–8°C): 30 hours	<1 CFU/100 mL	Daily	2 days
Ambient (recreational and ocean) water							
Total coliforms & <i>E. coli</i> MPN, Undiluted (8350)	Detection and enumeration of total coliforms and <i>E. coli</i> in ambient water	Ambient water	Collection in a 120 mL sterile Click Seal bottle	Refrigerated (2–8°C): 8 hours	<1 MPN/100 mL	Daily	1 day
Total coliforms & <i>E. coli</i> MPN, 1:10 dilution (8025)	Detection and enumeration of total coliforms and <i>E. coli</i> in ambient water	Ambient water	Collection in a 120 mL sterile Click Seal bottle	Refrigerated (2–8°C): 8 hours	<10 MPN/100 mL	Daily	1 day
Enterococci MPN, undiluted (8110)	Detection and enumeration of Enterococci in ambient water	Ambient water	Collection in a 120 mL sterile Click Seal bottle	Refrigerated (2–8°C): 8 hours	<1 MPN/100 mL	Daily	1 day

Test (Order code)	Description	Sample	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)
Enterococci MPN, 1:10 dilution (8010)	Detection and enumeration of Enterococci in ambient water	Ambient water	Collection in a 120 mL sterile Click Seal bottle	Refrigerated (2–8°C): 8 hours	<10 MPN/100 mL	Daily	1 day
Thermotolerant (fecal) coliforms MPN, A-1 (8910)	Enumeration of thermotolerant (fecal) coliforms in ambient water	Ambient water	Collection in a 120 mL sterile Click Seal bottle	Refrigerated (2–8°C): 8 hours	<1.8 MPN/100 mL	By appointment	1–2 days
Spa and swimming pool water							
Pseudomonas count (8050)	Detection and quantification of <i>Pseudomonas aeruginosa</i> in spa or pool water	Spa or pool water	Collection in a 100 mL Idexx bottle	Refrigerated (2–8°C): 30 hours	<1 MPN/100 mL	Daily	1 day
Heterotrophic plate count (8045)	Estimation of the number of live heterotrophic bacteria in spa or pool water	Spa or pool water	Collection in a 100 mL Idexx bottle	Refrigerated (2–8°C): 30 hours	<1 CFU/100 mL	Daily	2 days
Shellfish and shellfish growing waters							
NSSP Thermotolerant (fecal) coliforms, A-1, growing water (8710)	Enumeration of thermotolerant (fecal) coliforms by multiple tube fermentation (AOAC method)	Shellfish growing water	Collection in a 120 mL sterile Click Seal bottle	Refrigerated (2–8°C): 30 hours	<1.8 MPN/100 mL	By appointment	1–2 days
NSSP Total coliforms, process water (8720)	Enumeration of total coliforms by multiple tube fermentation (NSSP-modified method)	Shellfish process water	Collection in a sterile Nalgene bottle	Refrigerated (2–8°C): 30 hours	<1.1 MPN/100 mL	By appointment	4 days

Test (Order code)	Description	Sample	Collection	Storage/transport	Reference range	Testing schedule	TAT (business days)
NSSP Thermotolerant (fecal) coliforms, ocean shellfish (8770)	Enumeration of thermotolerant (fecal) coliforms by multiple tube fermentation (APHA method)	Ocean shellfish	Harvest of at least 12 shellfish (meat weight >200 g)	Refrigerated (0–4°C): 24 hours	<1.8 MPN/100 g	By appointment	3 days
NSSP Thermotolerant (fecal) coliforms, process shellfish (8780)	Enumeration of thermotolerant (fecal) coliforms by multiple tube fermentation (NSSP-modified method)	Process shellfish	Harvest of at least 12 shellfish (meat weight >200 g)	Refrigerated (0–4°C): 24 hours	<4 MPN/100 g	By appointment	3 days

CFU, colony forming unit; MPN, most probable number; TAT, turnaround time (estimated maximum time from specimen receipt to result, where the time is dependent upon day of receipt, testing schedule, and length of testing).

r. Water and shellfish specimen collection

1. Water collection in a 100 mL Idexx bottle

Sample

Water in Idexx bottle

2. Use only sterile containers supplied by the laboratory. Sample bottles can be picked up and dropped off at any of the Public Health Department locations in San Luis Obispo, Paso Robles, and Grover Beach.
3. Do not collect samples from a swivel head faucet. When taking water samples, remove the aerator; **flush the lines** by opening the cold water tap and running water for 2 to 3 minutes.
4. Carefully open the bottle — **do not touch the inside** of the bottle or lid.
5. **Do not rinse** out the bottle and **do not touch or dump** out the white powder.
6. Fill the bottle carefully to the **100 ml line** on the bottle (**DO NOT UNDERFILL** or **OVERFILL**), making sure the powder stays in the bottle. Close the cap tightly.
7. **Fill in all the requested fields** on the laboratory requisition (test request form). For guidance filling out the requisition, see Environmental Testing Requisition Instructions document or contact us. Create a sample ID number and write it on both the bottle and the requisition.
8. Water must begin cooling, to refrigerator temperature, immediately after collection. **Use cooler** with ice packs or equivalent for transport. Do not freeze.
9. Cost of testing is posted at www.slocounty.gov/PH-Lab, payable when the water sample is delivered to any Public Health Department. If testing shows the drinking water is unsafe to drink, a “Retest” sample will incur the same fee.
10. Please note on the laboratory requisition if the water test is for FHA, VA, or Cal-Vet Loans.



Idexx Water
Collection Bottle

Storage & Transport

Temperature: Refrigerated 2–8°C (36–46°F), not frozen.

Maximum Holding Time: 30 hours (time from collection to test set-up in laboratory incubator)

2. Water collection in a 120 mL sterile Click Seal bottle

Sample

Water in Click Seal bottle

1. Keep the sampling bottle unopened until right before filling.
2. For sampling hold the bottle near the base and plunge it neck downward below the surface. Once below the surface tilt the bottle to allow filling. During filling, the bottle should be pushed horizontally forward in a direction away from the hand to avoid contamination.
3. Do not touch the threads, inside, or lid interior of the bottle. Touching the interior of the bottle contaminates the sample and may affect results.
4. If sample/bottle is contaminated, collect a new sample.
 - a. The contaminated sample may be used as the temperature blank.
5. To allow for shaking, please do not fill the bottle completely full.



**Sterile Click Seal
Bottle**

Storage & Transport

Temperature: Refrigerated 2–8°C (36–46°F)

Maximum Holding Time: 8 or 30 hours depending on the test (time from collection to test set-up in laboratory incubator)

3. Water collection in a sterile Nalgene bottle

Sample

Water in sterile Nalgene bottle

1. Keep the sampling bottle unopened until right before filling.
2. For sampling hold the bottle near the base and plunge it neck downward below the surface. Once below the surface tilt the bottle to allow filling. During filling, the bottle should be pushed horizontally forward in a direction away from the hand to avoid contamination.
3. Do not touch the threads, inside, or lid interior of the bottle. Touching the interior of the bottle contaminates the sample and may affect results.
4. If sample/bottle is contaminated, collect a new sample.
 - a. The contaminated sample may be used as the temperature blank.
5. To allow for shaking, please do not fill the bottle completely full.



**Sterile Nalgene
Bottle**

Storage & Transport

Temperature: Refrigerated 2–8°C (36–46°F)

Maximum Holding Time: 30 hours (time from collection to test set-up in laboratory incubator)

IV. Reportable diseases

California Code of Regulations, Title 17, Section 2500, mandates that certain communicable and non-communicable diseases/conditions be reported to the local health authority by specified methods and time frames. The List of Reportable Diseases, which summarizes disease reporting requirements, may be downloaded from the [web](#), and freely copied.

In addition, California Code of Regulations, Title 17, Section 2505 requires laboratories to report laboratory testing results, including molecular and pathologic results, suggestive of diseases of public health importance to the local health department. Laboratories must report any initial findings as well as any subsequent findings. In addition, laboratories must report negative test results or findings when requested by the Department or a local health officer.

The specimens or isolates listed below must be submitted as soon as available to the local or state public health laboratory. The isolate or specimen submission must include the name, address, and date of birth of the person from whom the isolate or specimen was obtained, the patient identification number, the isolate or specimen accession number or other unique identifier, the date the isolate or specimen was obtained from the patient, the name address, and telephone number of the health care provider for whom such examination or test was performed, and the name, address, telephone number and laboratory director's name of the laboratory submitting the isolate or specimen.

Specimens:

- Malaria positive blood film slides
- *Neisseria meningitidis* eye specimens
- Shiga toxin-positive fecal broths
- Zika virus immunoglobulin M (IgM)-positive sera
- Drug resistant *Neisseria gonorrhoeae* isolates (cephalosporin or azithromycin only)
- *Listeria monocytogenes* isolates
- *Mycobacterium tuberculosis* isolates
- *Neisseria meningitidis* isolates from sterile sites
- Salmonella isolates (see section 2612 for additional reporting requirements)
- Shiga toxin-producing *Escherichia coli* (STEC) isolates, including O157 and non-O157 strains
- *Shigella* isolates